

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021020\
 Data File : BM024827.D
 Acq On : 11 Feb 2020 02:29
 Operator : CG/JU
 Sample : L1402-20
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6X9

Quant Time: Feb 11 03:49:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 07 07:38:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	295407	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.16	136	1157884	20.00	ng/ul	-0.01
36) Acenaphthene-d10	14.05	164	754797	20.00	ng/ul	-0.01
62) Phenanthrene-d10	16.81	188	1609996	20.00	ng/ul	0.00
78) Chrysene-d12	21.02	240	1562023	20.00	ng/ul	-0.01
86) Perylene-d12	23.12	264	1609855	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.01	96	41962	6.83	ng/uL	0.00
5) Phenol-d5	6.60	99	713711	36.37	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	6.75	67	425023	38.35	ng/ul	-0.01
9) 2-Chlorophenol-d4	6.94	132	648065	36.86	ng/ul	-0.01
13) 4-Methylphenol-d8	8.12	113	600635	36.27	ng/ul	-0.01
19) Nitrobenzene-d5	8.54	128	317139	37.88	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.26	143	381273	38.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.79	165	678019	33.97	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.30	131	850115	45.54	ng/ul	-0.01
44) Dimethylphthalate-d6	13.48	166	2044138	35.88	ng/ul	0.00
47) Acenaphthylene-d8	13.74	160	2486641	37.37	ng/ul	-0.01
52) 4-Nitrophenol-d4	14.27	143	294967	31.86	ng/ul	-0.01
58) Fluorene-d10	15.06	176	1789053	35.46	ng/ul	-0.01
63) 4,6-Dinitro-2-methylphenol	15.19	200	309730	29.51	ng/ul	0.00
71) Anthracene-d10	16.91	188	2674035	36.38	ng/ul	0.00
79) Pyrene-d10	19.22	212	2900497	37.12	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.99	264	3000411	37.11	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.53	163	102928	1.732	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021020\
Data File : BM024827.D
Acq On : 11 Feb 2020 02:29
Operator : CG/JU
Sample : L1402-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB6X9

Quant Time: Feb 11 03:49:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 07 07:38:13 2020
Response via : Initial Calibration

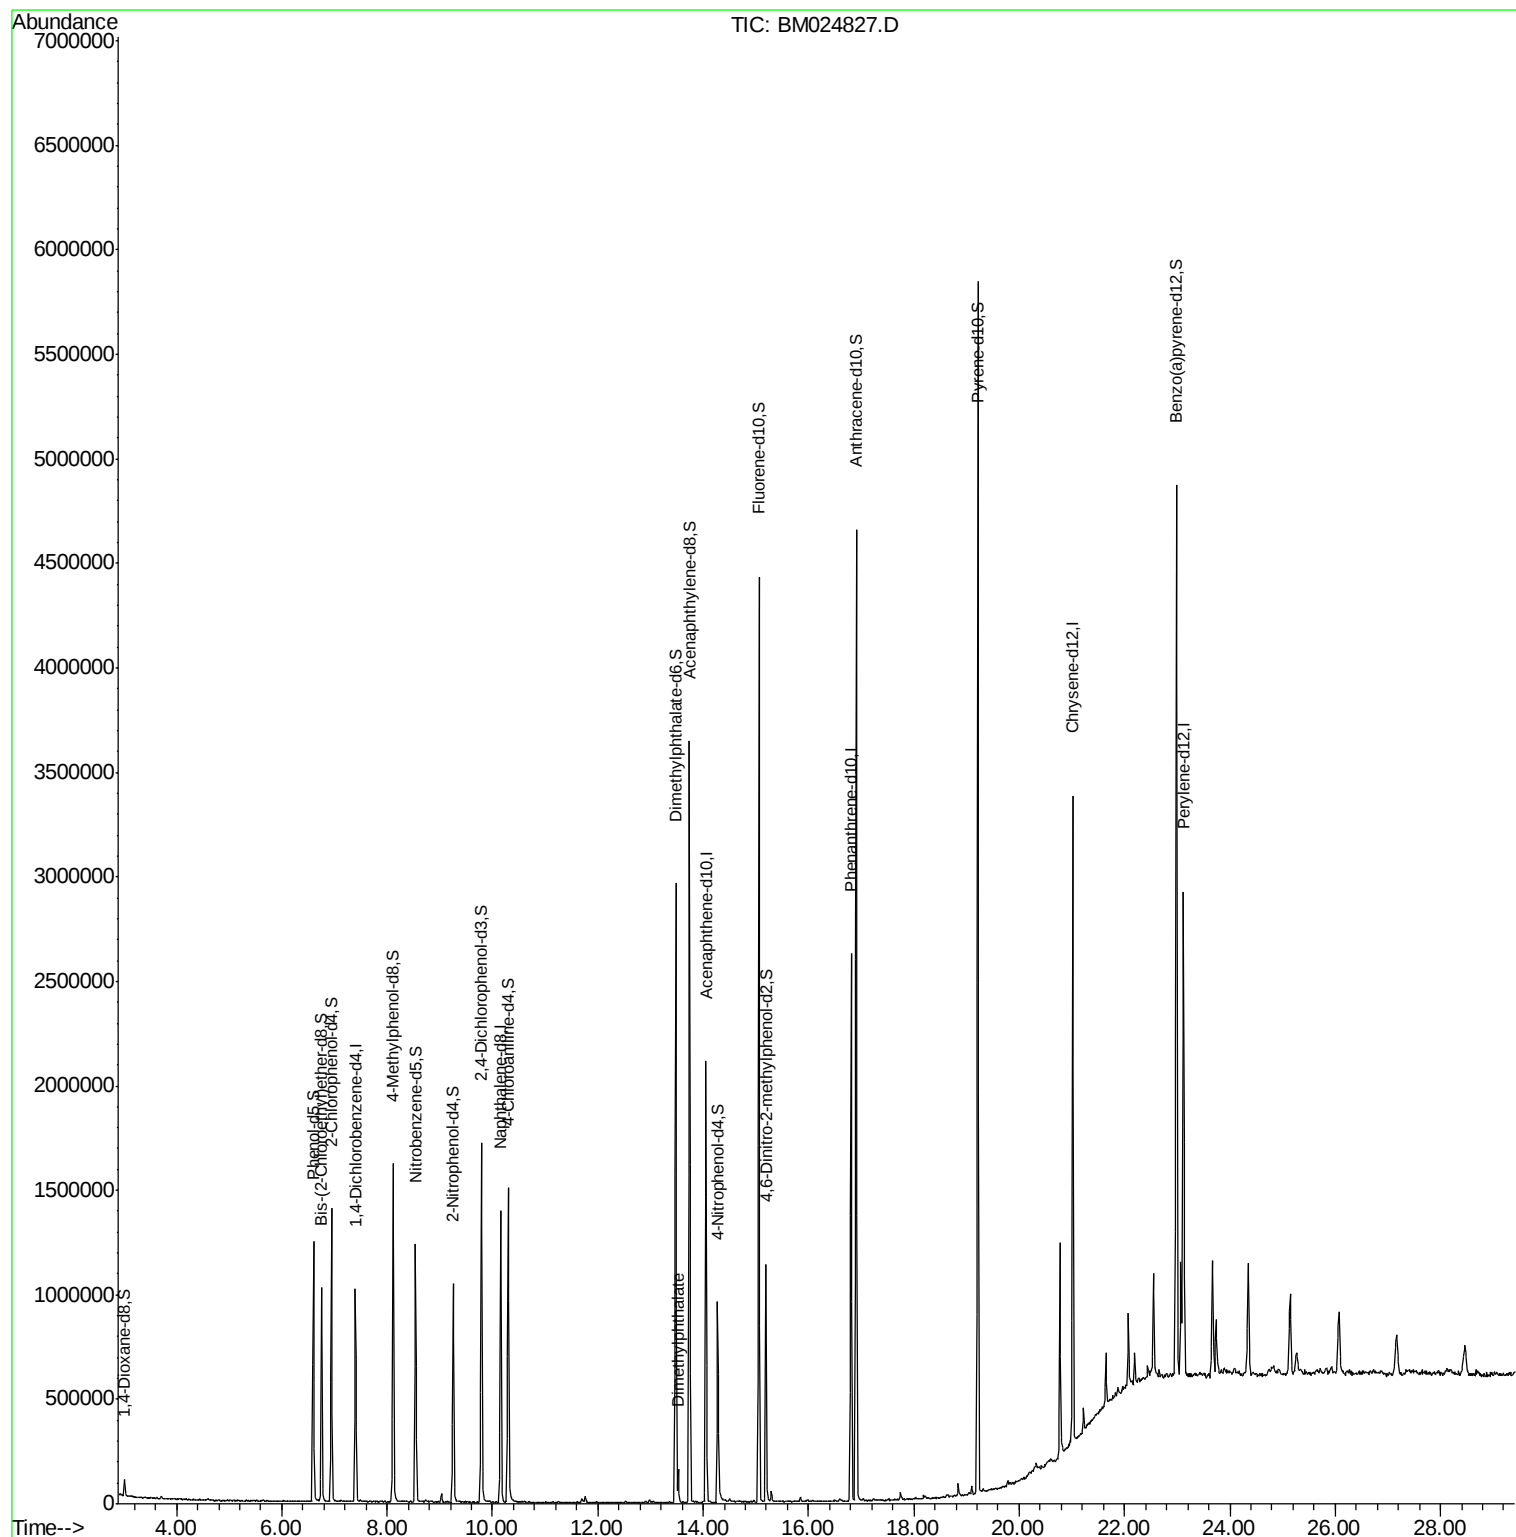

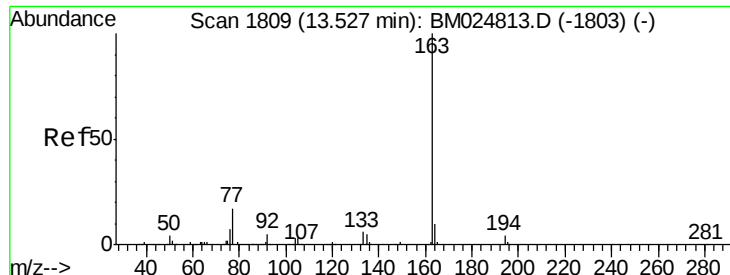

#45

Dimethylphthalate

Concen: 1.732 ng/ul

RT: 13.53 min Scan# 1809

Delta R.T. -0.01 min

Lab File: BM024827.D

Acq: 11 Feb 2020 02:29

Instrument :

BNA_M

ClientSampleId :

CB6X9



Tot Ion:163 Resp: 102928

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 10.3 8.2 12.2

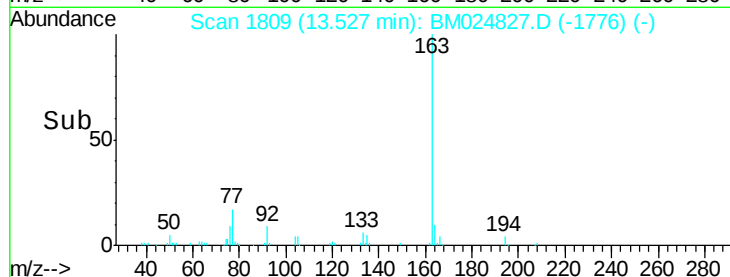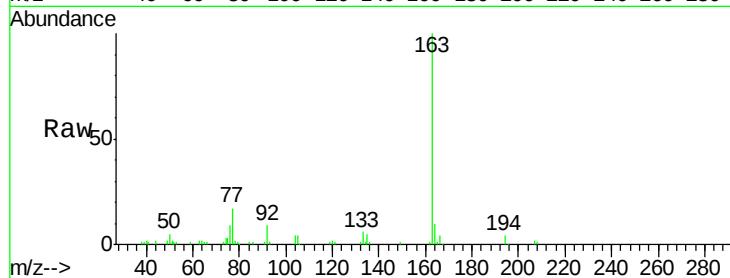

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

