

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021121\
 Data File : BM028723.D
 Acq On : 11 Feb 2021 22:14
 Operator : CG/JU
 Sample : M1375-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BJ5

Quant Time: Feb 11 23:47:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Feb 11 16:46:31 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.89	152	26084	20.00	ng/ul	0.00
18) Naphthalene-d8	10.70	136	101243	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.54	164	54803	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.27	188	107562	20.00	ng/ul	0.00
78) Chrysene-d12	21.42	240	106106	20.00	ng/ul	0.00
86) Perylene-d12	23.66	264	110753	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.20	96	574	0.93	ng/uL	0.00
5) Phenol-d5	7.06	99	11868	5.33	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.22	67	25679	18.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.42	132	34045	17.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.61	113	22192	12.34	ng/ul	0.00
19) Nitrobenzene-d5	9.06	128	17356	20.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.79	143	19236	20.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.32	165	39103	22.68	ng/ul	0.00
29) 4-Chloroaniline-d4	10.85	131	4888	2.44	ng/ul	0.00
44) Dimethylphthalate-d6	13.95	166	102823	23.63	ng/ul	0.00
47) Acenaphthylene-d8	14.23	160	125006	22.49	ng/ul	0.00
52) 4-Nitrophenol-d4	14.76	143	3838	4.71	ng/ul	0.00
58) Fluorene-d10	15.53	176	84482	22.46	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.66	200	15088	20.38	ng/ul	0.00
71) Anthracene-d10	17.37	188	138942	25.09	ng/ul	0.00
79) Pyrene-d10	19.65	212	144999	23.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.52	264	155931	24.81	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	14.00	163	17159	3.890	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021121\
Data File : BM028723.D
Acq On : 11 Feb 2021 22:14
Operator : CG/JU
Sample : M1375-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BJ5

Quant Time: Feb 11 23:47:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Feb 11 16:46:31 2021
Response via : Initial Calibration

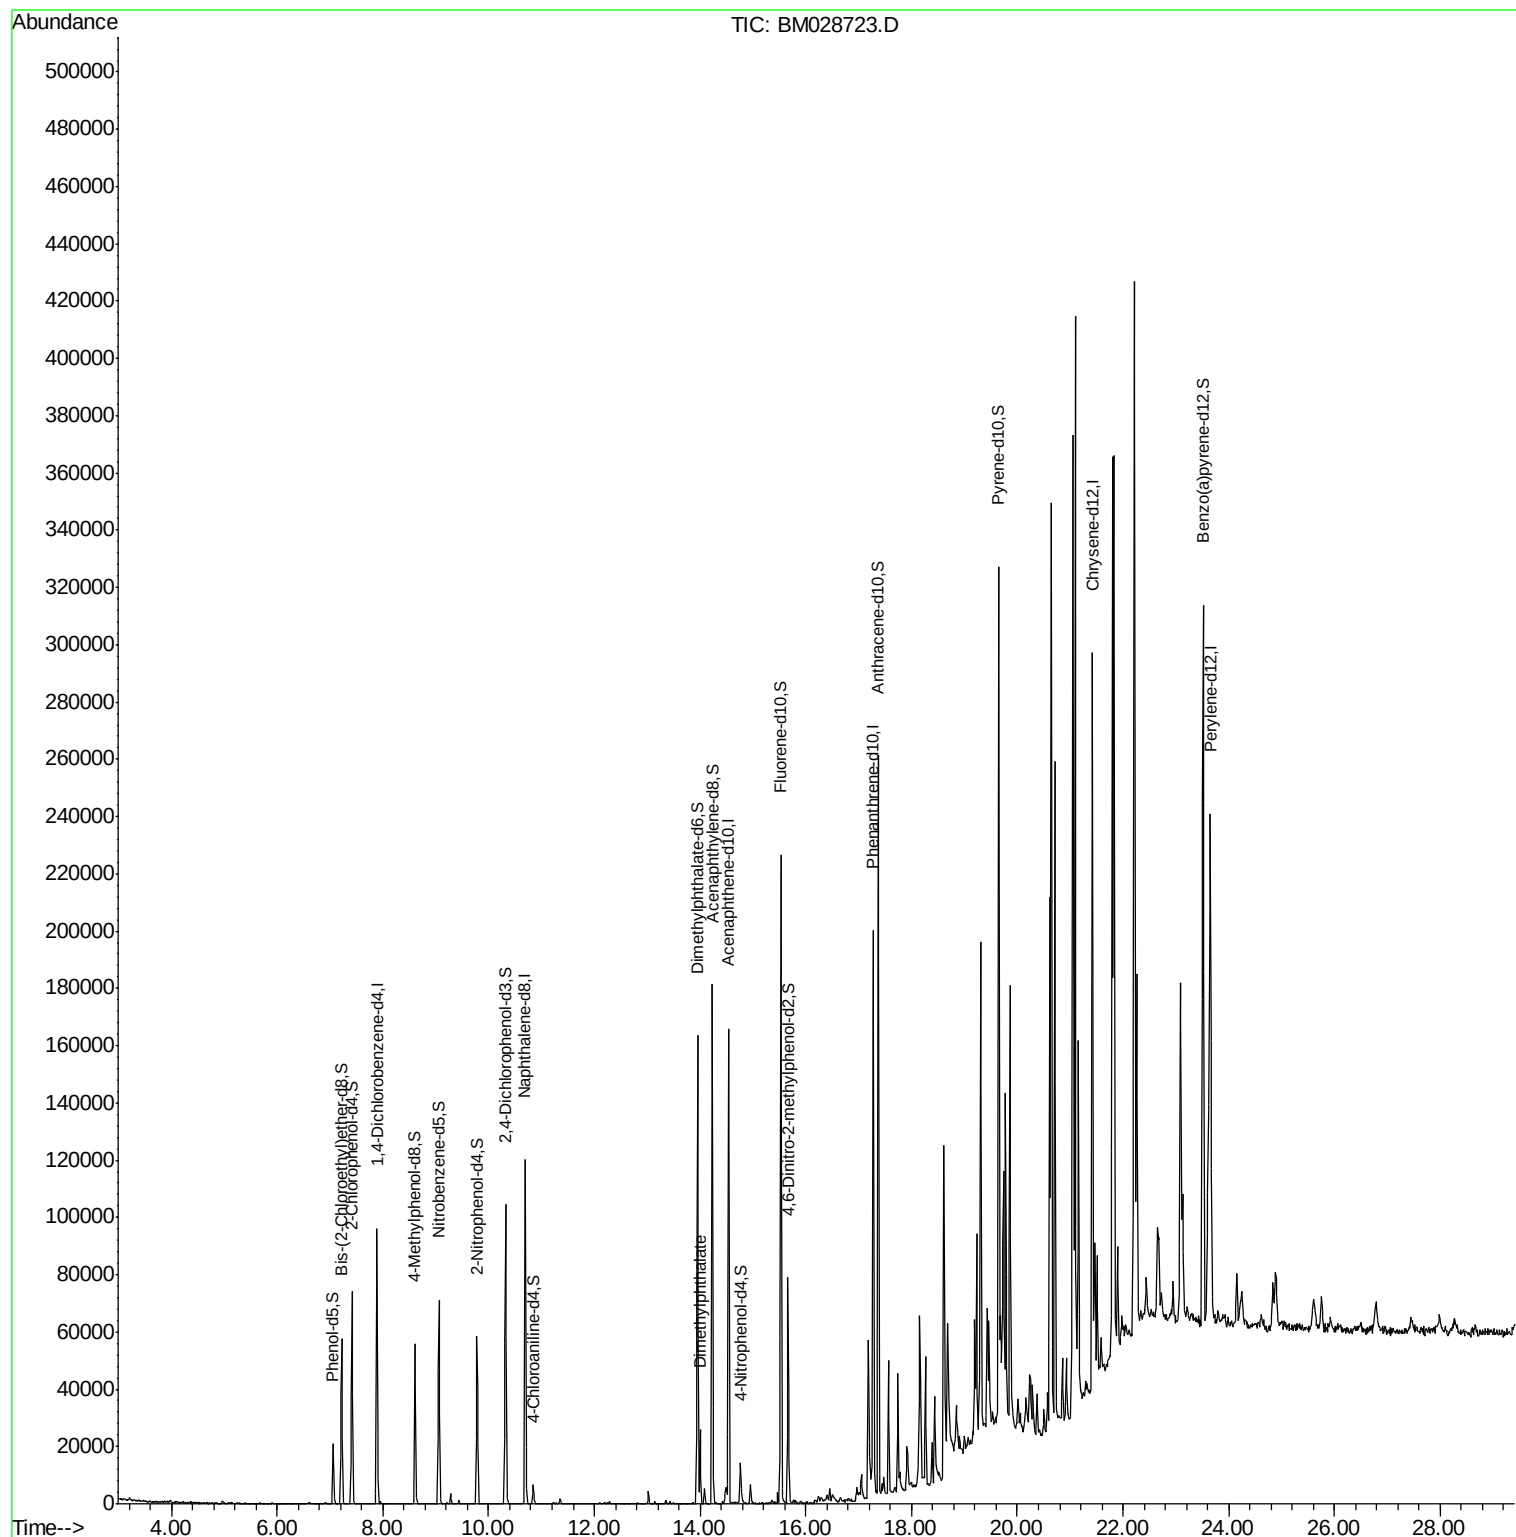


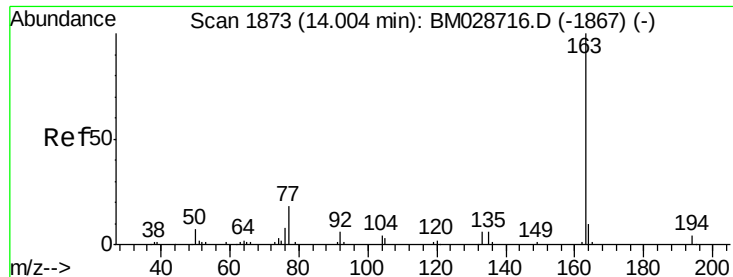

#45
 Dimethylphthalate
 Concen: 3.890 ng/ul
 RT: 14.00 min Scan# 1872
 Delta R.T. -0.01 min
 Lab File: BM028723.D
 Acq: 11 Feb 2021 22:14

Instrument :
 BNA_M
 ClientSampleId :
 C0BJ5

Tot Ion:163 Resp: 17159
 Ion Ratio Lower Upper
 163 100
 194 4.7 3.3 4.9
 164 9.9 8.2 12.2

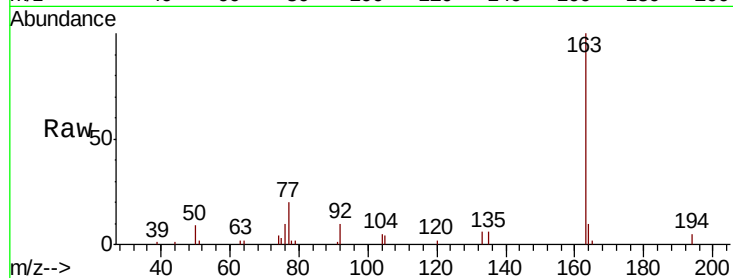

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

