

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021121\
 Data File : BM028717.D
 Acq On : 11 Feb 2021 18:37
 Operator : CG/JU
 Sample : PB134593BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK93

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.199	32	36	42	rBV	7376	9582	1.79%	0.161%
2	3.975	165	168	170	rBV	939	1237	0.23%	0.021%
3	7.057	686	692	706	rBB	122323	188669	35.29%	3.166%
4	7.222	714	720	731	rBB	90474	143801	26.90%	2.413%
5	7.416	747	753	762	rBV	131421	200518	37.50%	3.365%
6	7.886	827	833	842	rBB	105520	162496	30.39%	2.727%
7	8.610	950	956	967	rBB	143896	225106	42.10%	3.778%
8	9.063	1027	1033	1042	rBV	109477	175687	32.86%	2.948%
9	9.786	1150	1156	1164	rBB	89065	145460	27.21%	2.441%
10	10.322	1241	1247	1258	rBB	142482	224651	42.02%	3.770%
11	10.698	1304	1311	1320	rBB	142294	227624	42.57%	3.820%
12	10.839	1329	1335	1349	rBB	136824	226838	42.43%	3.807%
13	12.286	1578	1581	1585	rBB2	1441	1905	0.36%	0.032%
14	13.957	1859	1865	1871	rBV	210223	292158	54.64%	4.903%
15	14.239	1906	1913	1923	rBV	264668	380325	71.13%	6.383%
16	14.545	1959	1965	1972	rBB	187756	273961	51.24%	4.598%
17	14.757	1996	2001	2014	rBV	88378	128445	24.02%	2.156%
18	15.533	2127	2133	2140	rBV	318586	436757	81.69%	7.330%
19	15.668	2151	2156	2162	rBV	87318	114940	21.50%	1.929%
20	15.774	2170	2174	2177	rVB2	1884	2055	0.38%	0.034%
21	17.280	2424	2430	2437	rVB	202015	286370	53.56%	4.806%
22	17.374	2440	2446	2455	rVV	324109	446094	83.43%	7.486%
23	18.151	2575	2578	2584	rVB2	2091	2412	0.45%	0.040%
24	18.703	2670	2672	2674	rBV2	468	538	0.10%	0.009%
25	19.021	2723	2726	2729	rBV3	413	641	0.12%	0.011%
26	19.292	2768	2772	2776	rBV	2374	3118	0.58%	0.052%
27	19.427	2793	2795	2798	rBV3	1345	993	0.19%	0.017%
28	19.545	2810	2815	2819	rVV2	2026	3103	0.58%	0.052%
29	19.656	2828	2834	2840	rBV	382578	492069	92.03%	8.258%
30	21.427	3130	3135	3140	rBV	257759	307516	57.52%	5.161%
31	23.521	3485	3491	3501	rVB	301912	534664	100.00%	8.973%
32	23.662	3509	3515	3523	rVB2	179392	318934	59.65%	5.352%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021121\
Data File : BM028717.D
Acq On : 11 Feb 2021 18:37
Operator : CG/JU
Sample : PB134593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK93

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 5958667

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021121\
Data File : BM028717.D
Acq On : 11 Feb 2021 18:37
Operator : CG/JU
Sample : PB134593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK93

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

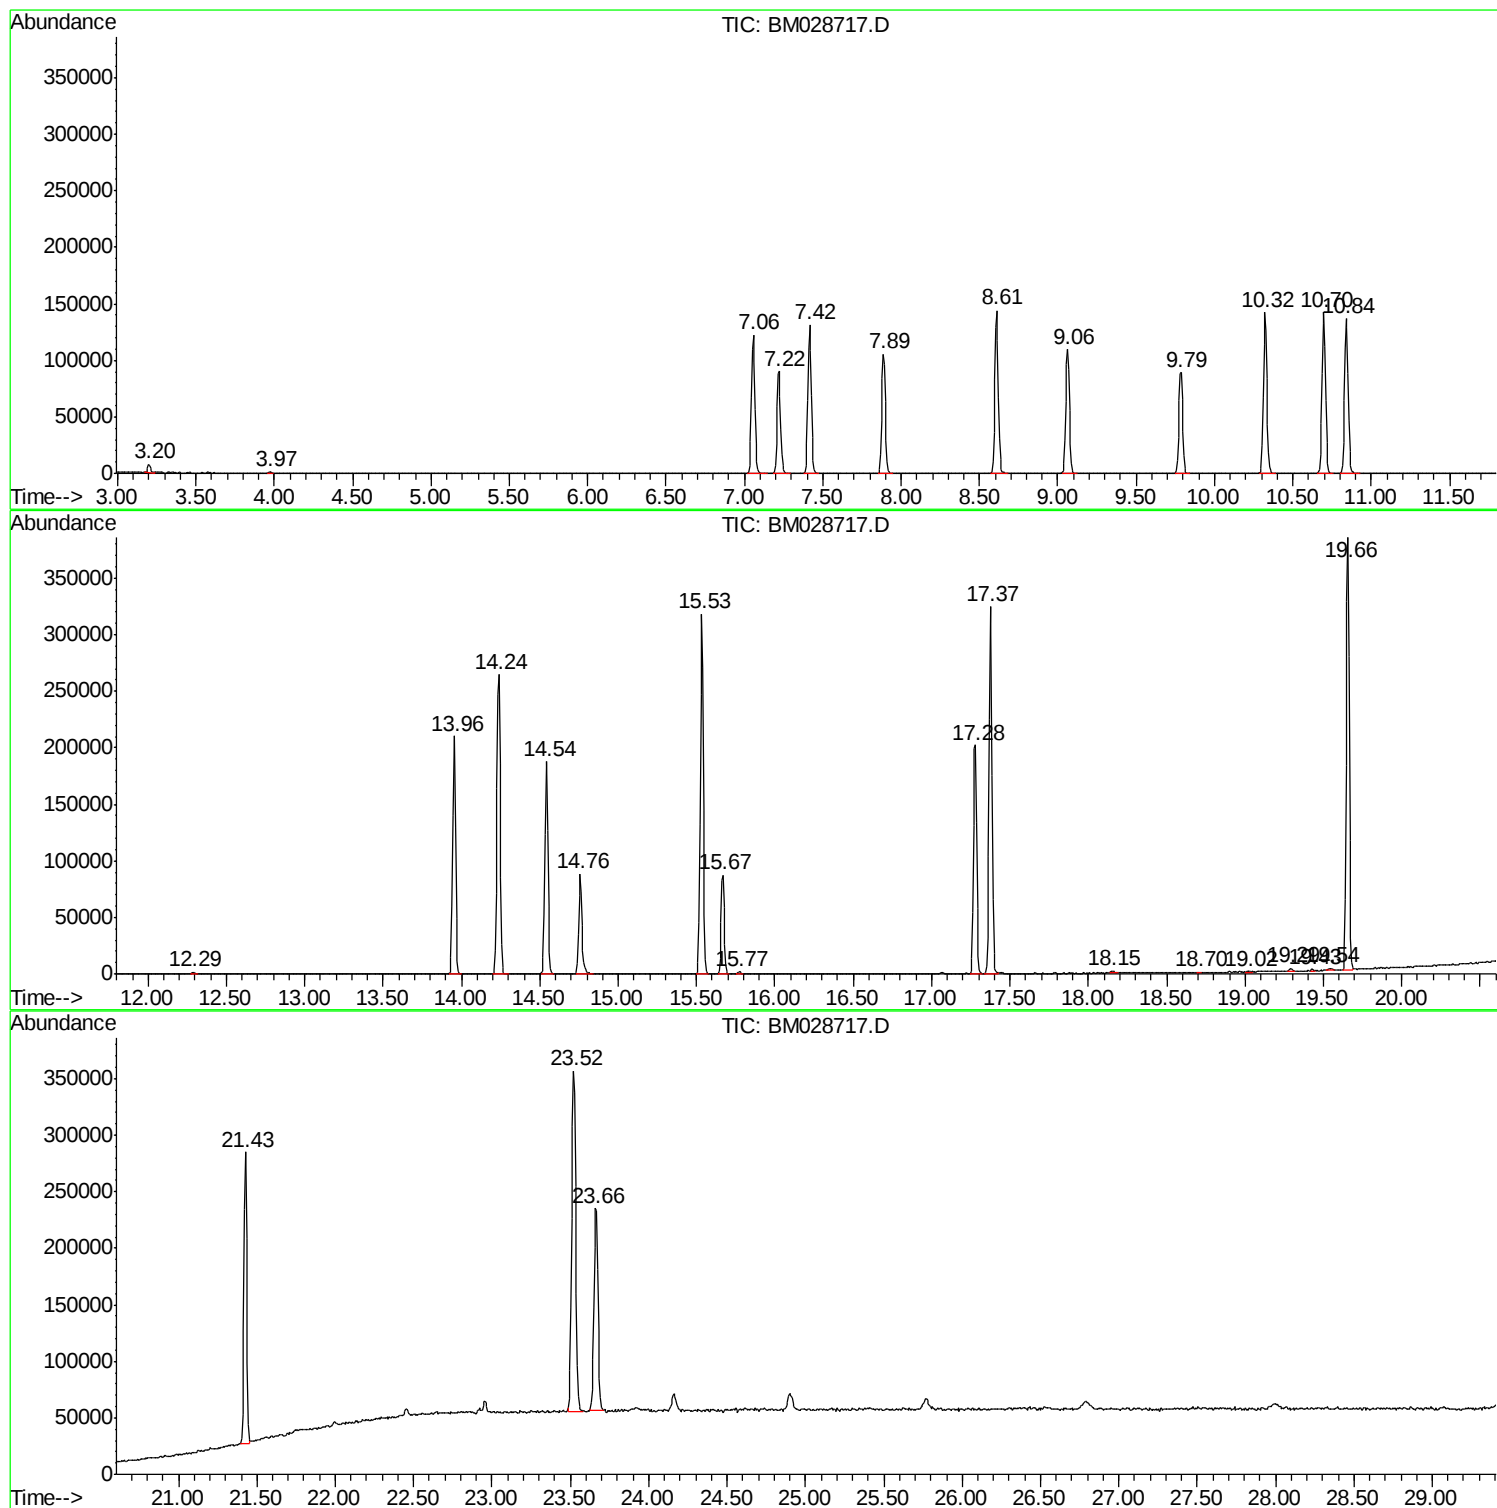

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021121\
Data File : BM028717.D
Acq On : 11 Feb 2021 18:37
Operator : CG/JU
Sample : PB134593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK93

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021121\
Data File : BM028717.D
Acq On : 11 Feb 2021 18:37
Operator : CG/JU
Sample : PB134593BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK93

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc