


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021121\
 Data File : BM028715.D
 Acq On : 11 Feb 2021 15:11
 Operator : CG/JU
 Sample : DFTPP27
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP27

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011621MA.M
 Title : SVOA CALIBRATION
 Last Update : Thu Feb 11 16:46:31 2021

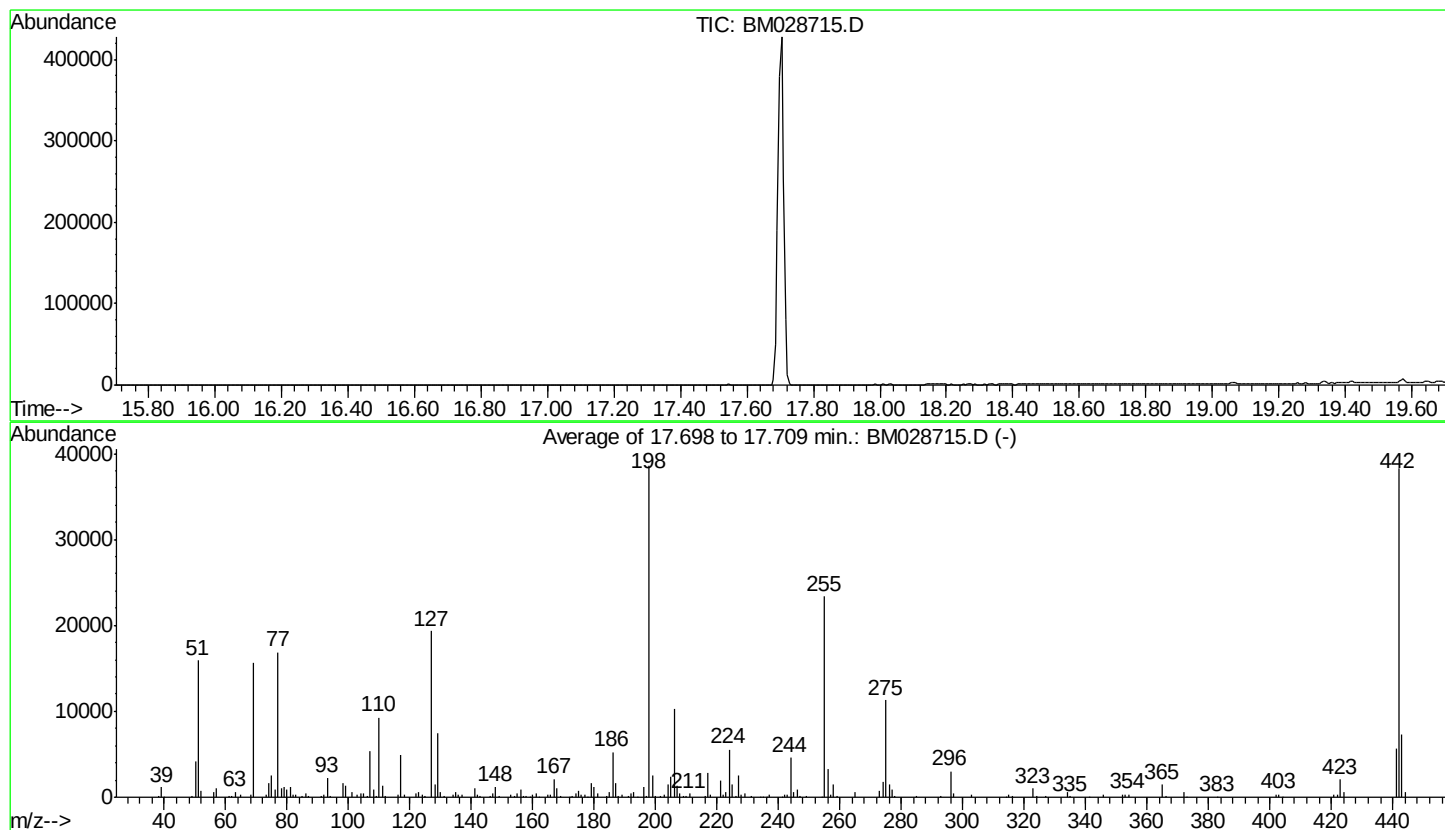

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	15915	PASS
68	69	0.00	2	1.8	276	PASS
69	198	0.00	100	40.4	15576	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.1	19314	PASS
197	198	0.00	2	0.4	167	PASS
198	198	100	100	100.0	38589	PASS
199	198	5	9	6.5	2525	PASS
275	198	10	60	29.2	11280	PASS
365	198	1	100	3.7	1442	PASS
441	198	0.01	100	14.7	5670	PASS
442	198	50	100	99.0	38216	PASS
443	442	15	24	19.3	7376	PASS

Scan 2496 (17.668 min): BM028715.D
DFTPP27

m/z	Abundance
44.00	309.0
207.00	261.0

Instrument :
BNA_M
ClientSampleId :
DFTPP27

m/z	Abundance
38.00	327.0
39.00	1419.0
43.90	274.0
49.00	221.0
50.10	5095.0
51.10	19280.0
52.00	1022.0
56.00	653.0
57.00	1395.0
60.90	240.0
61.90	247.0
63.00	792.0
65.00	382.0
68.00	337.0
69.00	18704.0
73.00	310.0
74.00	2058.0
75.00	2942.0
76.10	1109.0
77.10	20440.0
78.00	1407.0
79.00	1362.0
80.00	1151.0
81.00	1522.0
82.00	342.0
82.90	322.0
85.00	263.0
85.90	453.0
87.00	244.0
91.00	348.0
92.00	443.0
93.00	2652.0
94.00	159.0
98.00	2016.0
99.00	1565.0
100.90	706.0
103.00	272.0
104.00	518.0
105.00	466.0
105.90	192.0
107.00	6116.0
108.00	1036.0
109.10	204.0
110.00	10767.0
111.00	1687.0
112.00	200.0
116.00	467.0
117.00	5713.0
118.00	438.0
121.90	461.0
122.90	583.0
124.00	374.0
124.90	299.0
127.00	22544.0
128.00	1795.0
129.00	8424.0
130.00	688.0
131.00	165.0
133.90	242.0
135.00	640.0
135.90	249.0
137.00	328.0
141.00	1132.0
142.00	369.0
142.90	244.0
146.00	165.0
147.00	589.0
148.00	1482.0
148.90	269.0
152.90	380.0
153.90	269.0
155.00	577.0
156.00	944.0
157.00	187.0
157.90	208.0
159.00	164.0
160.00	375.0
160.90	537.0
161.90	163.0
165.00	379.0
165.90	292.0
167.00	2435.0
168.00	1232.0
169.10	152.0
173.00	170.0
174.00	471.0
175.00	856.0
175.90	266.0
176.90	335.0
179.00	1817.0
180.00	1231.0
180.90	462.0

Instrument :
BNA_M
ClientSampleId :
DFTPP27

184.00	176.0
185.00	717.0
186.00	5480.0
187.00	1582.0
188.00	174.0
188.90	359.0
190.90	225.0
191.90	534.0
193.00	583.0
194.00	160.0
196.00	1099.0
197.10	341.0
198.00	42224.0
198.90	2785.0
200.00	221.0
201.50	209.0
202.90	360.0
204.00	1635.0
205.00	2784.0
206.00	10950.0
207.00	1715.0
208.00	459.0
210.00	201.0
211.00	402.0
216.00	278.0
217.00	3048.0
217.90	321.0
221.00	1905.0
222.90	604.0
224.00	5779.0
225.00	1679.0
226.00	192.0
227.00	2616.0
227.90	380.0
229.00	561.0
231.00	342.0
236.00	152.0
237.00	338.0
241.00	158.0
242.00	271.0
243.00	357.0
244.10	4689.0
245.00	713.0
246.00	801.0
247.00	192.0
249.00	180.0
254.10	235.0
255.00	23536.0
256.00	3386.0
257.00	269.0
258.00	1389.0
259.00	209.0
265.00	569.0
273.00	750.0
274.00	1795.0
275.00	11256.0
276.00	1608.0
277.00	883.0
285.00	164.0
293.00	197.0
296.00	3048.0
297.00	436.0
303.00	310.0
314.90	313.0
316.00	180.0
323.00	944.0
324.00	203.0
334.00	651.0
341.00	150.0
346.00	185.0
352.00	219.0
352.90	266.0
354.00	355.0
365.00	1295.0
366.00	154.0
372.00	503.0
402.00	211.0
402.90	284.0
421.00	217.0
421.90	280.0
423.00	1817.0
424.00	622.0
441.00	4587.0
442.00	31872.0
443.00	6419.0
443.90	641.0

Instrument :
BNA_M
ClientSampleId :
DFTPP27

m/z	Abundance
38.00	250.0
39.10	1348.0
40.00	164.0
44.00	276.0
49.10	178.0
50.10	5061.0
51.00	18872.0
52.00	913.0
56.00	582.0
57.00	1268.0
61.00	211.0
62.00	296.0
63.00	780.0
65.00	426.0
68.00	331.0
69.00	18464.0
73.00	315.0
74.00	1886.0
75.00	3235.0
76.00	1092.0
77.10	20312.0
78.00	1230.0
79.00	1488.0
80.00	1103.0
81.00	1519.0
81.90	390.0
83.00	301.0
84.90	286.0
86.00	482.0
87.00	242.0
91.00	322.0
92.00	389.0
93.00	2643.0
93.90	159.0
98.00	1849.0
99.00	1435.0
101.00	869.0
102.90	313.0
104.00	539.0
105.00	440.0
106.00	171.0
107.00	6609.0
108.00	980.0
108.90	177.0
110.00	11265.0
111.00	1682.0
111.90	271.0
116.00	345.0
117.00	5676.0
118.00	420.0
122.00	449.0
123.00	697.0
123.90	313.0
125.00	264.0
127.00	23200.0
128.00	1809.0
129.00	8925.0
129.90	721.0
131.00	194.0
133.90	297.0
135.00	747.0
135.90	310.0
137.00	472.0
140.90	1209.0
142.00	351.0
142.90	270.0
146.00	241.0
147.00	631.0
148.00	1427.0
148.90	306.0
152.90	349.0
153.90	350.0
155.00	614.0
156.00	997.0
157.10	195.0
157.90	184.0
160.00	394.0
161.00	701.0
165.00	438.0
166.00	372.0
167.00	2609.0
168.00	1271.0
168.90	192.0
171.90	218.0
173.00	242.0
174.00	516.0
175.00	891.0
175.90	273.0
176.90	499.0
178.00	160.0
178.90	1904.0
180.00	1451.0

Instrument :
BNA_M
ClientSampleId :
DFTPP27

181.00	613.0
184.00	160.0
185.00	758.0
186.00	6141.0
187.00	2009.0
187.90	206.0
189.00	422.0
191.00	212.0
191.90	672.0
193.00	719.0
195.90	1475.0
198.00	46368.0
199.00	3017.0
199.90	218.0
201.40	214.0
203.00	302.0
204.00	1928.0
205.00	2781.0
206.00	12583.0
207.00	1793.0
208.00	469.0
209.00	260.0
210.00	242.0
211.00	464.0
216.00	267.0
217.00	3303.0
218.00	457.0
221.00	2375.0
221.90	431.0
223.00	752.0
224.00	6876.0
225.00	1702.0
226.00	182.0
227.00	3001.0
228.00	363.0
228.90	553.0
231.00	238.0
233.90	218.0
235.00	175.0
237.00	277.0
242.00	387.0
243.00	459.0
244.00	5479.0
245.10	755.0
246.00	1150.0
247.00	223.0
248.90	216.0
255.00	28728.0
256.00	4074.0
257.00	326.0
258.00	1856.0
259.00	275.0
265.00	701.0
272.90	781.0
274.00	2170.0
275.00	13620.0
276.00	1764.0
277.00	1113.0
277.90	172.0
284.90	180.0
292.90	245.0
296.00	3751.0
296.90	522.0
303.00	438.0
314.10	181.0
315.00	428.0
316.00	272.0
323.00	1289.0
324.00	167.0
327.00	240.0
334.00	788.0
334.90	226.0
345.90	272.0
352.00	366.0
353.00	223.0
354.00	373.0
365.00	1799.0
366.00	270.0
372.00	653.0
372.90	159.0
383.00	215.0
402.00	275.0
402.90	428.0
403.90	196.0
420.90	456.0
421.90	396.0
423.00	2403.0
424.00	665.0
441.00	7124.0
442.00	45752.0
443.00	8877.0
444.00	821.0

Instrument :
BNA_M
ClientSampleId :
DFTPP27

m/z	Abundance
39.00	677.0
43.90	264.0
50.10	2467.0
51.00	9594.0
52.00	456.0
56.00	358.0
57.00	658.0
63.00	357.0
65.00	170.0
68.00	162.0
69.00	9562.0
73.00	198.0
74.00	1090.0
75.00	1487.0
76.00	440.0
77.10	9963.0
78.00	695.0
79.00	734.0
80.00	557.0
81.00	756.0
82.00	205.0
83.00	184.0
85.90	219.0
92.00	228.0
93.00	1437.0
98.00	1093.0
99.00	865.0
100.90	431.0
102.90	153.0
104.00	299.0
104.90	244.0
107.00	3417.0
108.00	510.0
110.00	5909.0
111.00	858.0
116.00	232.0
117.00	3236.0
117.90	270.0
122.00	249.0
123.00	385.0
124.00	159.0
127.00	12200.0
128.00	980.0
129.00	5073.0
130.00	457.0
133.90	156.0
135.00	417.0
135.90	151.0
136.90	251.0
141.00	668.0
142.00	240.0
146.90	337.0
148.00	754.0
153.00	258.0
155.00	386.0
156.00	569.0
160.00	161.0
161.00	338.0
165.00	276.0
165.80	150.0
167.00	1437.0
168.00	814.0
173.00	180.0
173.90	274.0
175.00	499.0
175.90	187.0
176.90	234.0
178.90	1039.0
180.00	699.0
181.00	347.0
185.00	470.0
186.00	4079.0
187.00	1179.0
188.90	258.0
191.90	308.0
193.00	349.0
196.00	827.0
197.10	161.0
198.00	27176.0
199.00	1773.0
203.00	195.0
204.00	1025.0
205.00	1793.0
206.00	7431.0
207.00	1373.0
208.00	345.0
211.00	298.0
217.00	1943.0
218.00	268.0
221.00	1422.0
221.90	260.0
223.00	418.0

Instrument :
BNA_M
ClientSampleId :
DFTPP27

224.00	4102.0
225.00	986.0
227.00	1792.0
227.90	243.0
229.00	411.0
237.00	164.0
242.00	207.0
243.00	227.0
244.00	3525.0
245.00	438.0
245.90	579.0
246.90	150.0
255.00	17792.0
256.00	2594.0
257.00	208.0
258.00	1080.0
265.00	464.0
272.90	624.0
274.00	1499.0
275.00	8965.0
276.00	1040.0
277.00	730.0
277.90	163.0
292.80	168.0
296.00	2241.0
297.00	311.0
303.00	258.0
315.00	276.0
323.00	850.0
323.90	165.0
326.80	161.0
334.00	518.0
335.00	180.0
345.90	251.0
352.00	244.0
353.00	249.0
354.00	306.0
365.00	1232.0
372.00	544.0
401.90	205.0
402.90	326.0
421.00	265.0
421.90	359.0
422.90	1990.0
424.00	513.0
441.00	5300.0
442.00	37024.0
443.00	6833.0
444.00	548.0

Instrument :
BNA_M
ClientSampleId :
DFTPP27