
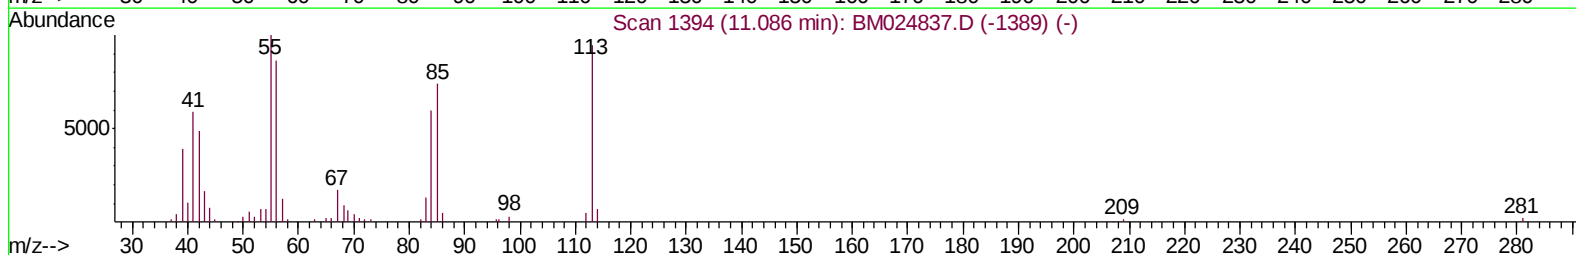
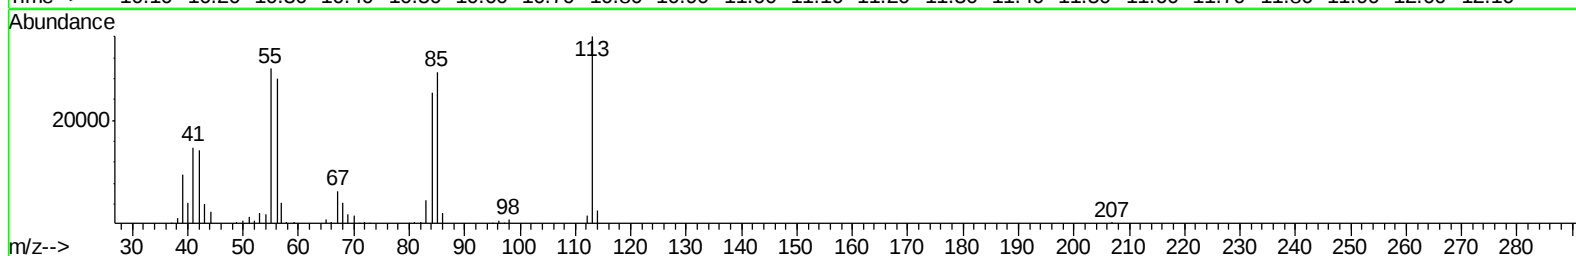


Data File : BM024856.D
Acq On : 13 Feb 2020 15:01
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 14 05:58:36 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 12 04:40:07 2020
Response via : Initial Calibration

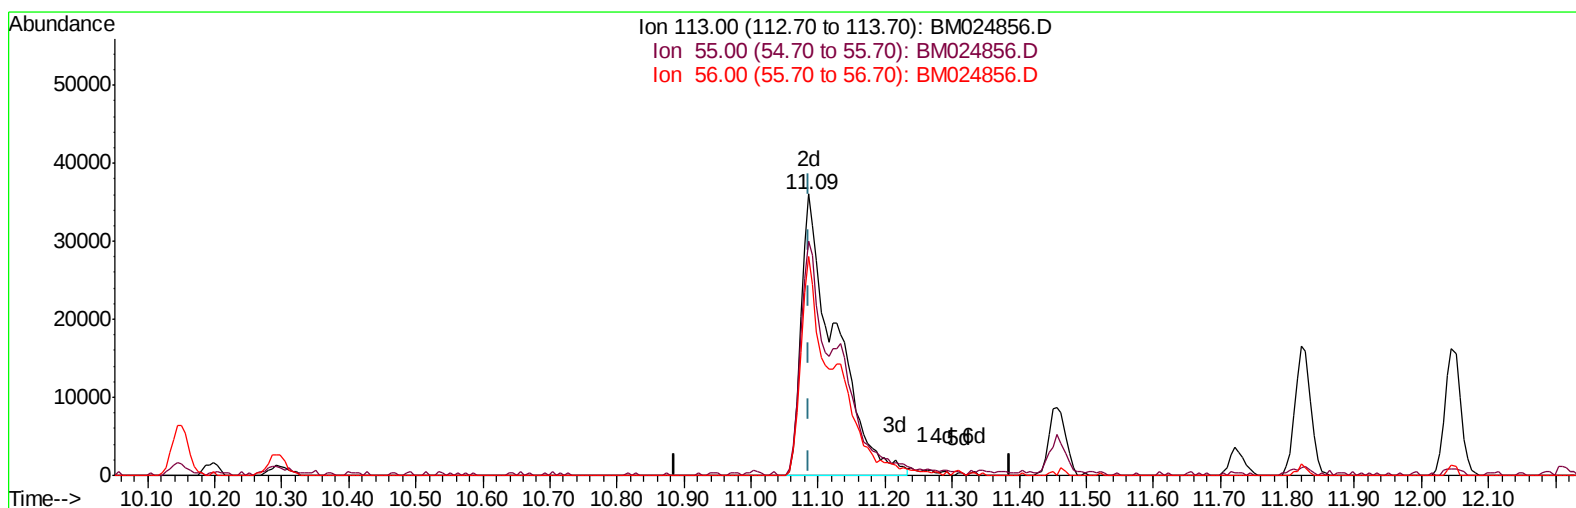

TIC: BM024856.D

(32) Caprolactam

11.086min (-0.000) 19.22ng/ul m

response 126993

Ion	Exp%	Act%
113.00	100	100
55.00	107.70	82.99#
56.00	89.90	77.78
0.00	0.00	0.00