
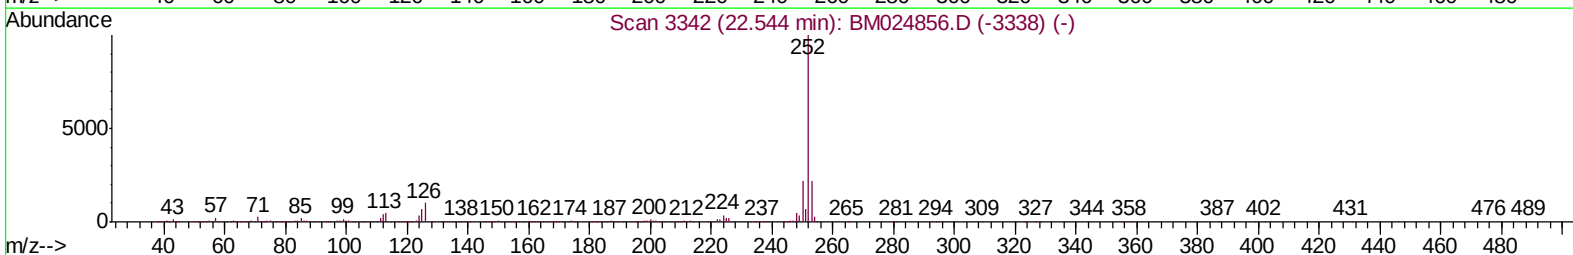
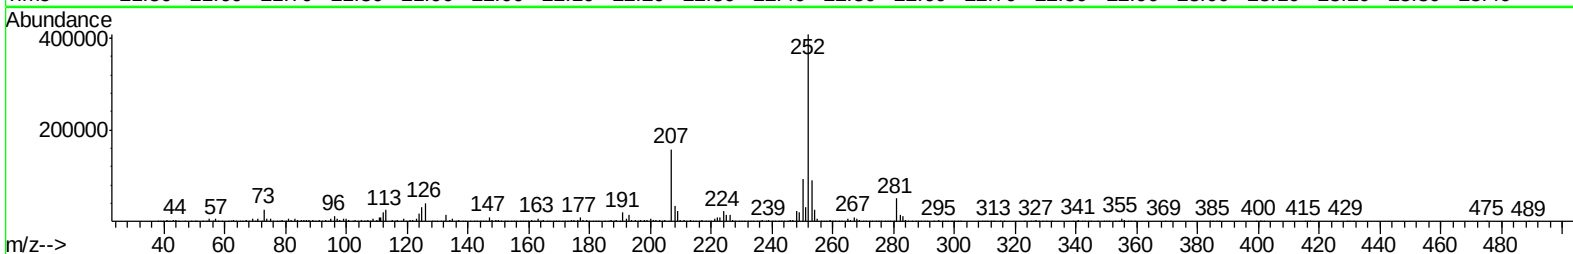


Data File : BM024864.D
Acq On : 13 Feb 2020 20:26
Operator : CG/JU
Sample : L1404-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Feb 14 06:02:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 14 05:59:53 2020
Response via : Initial Calibration

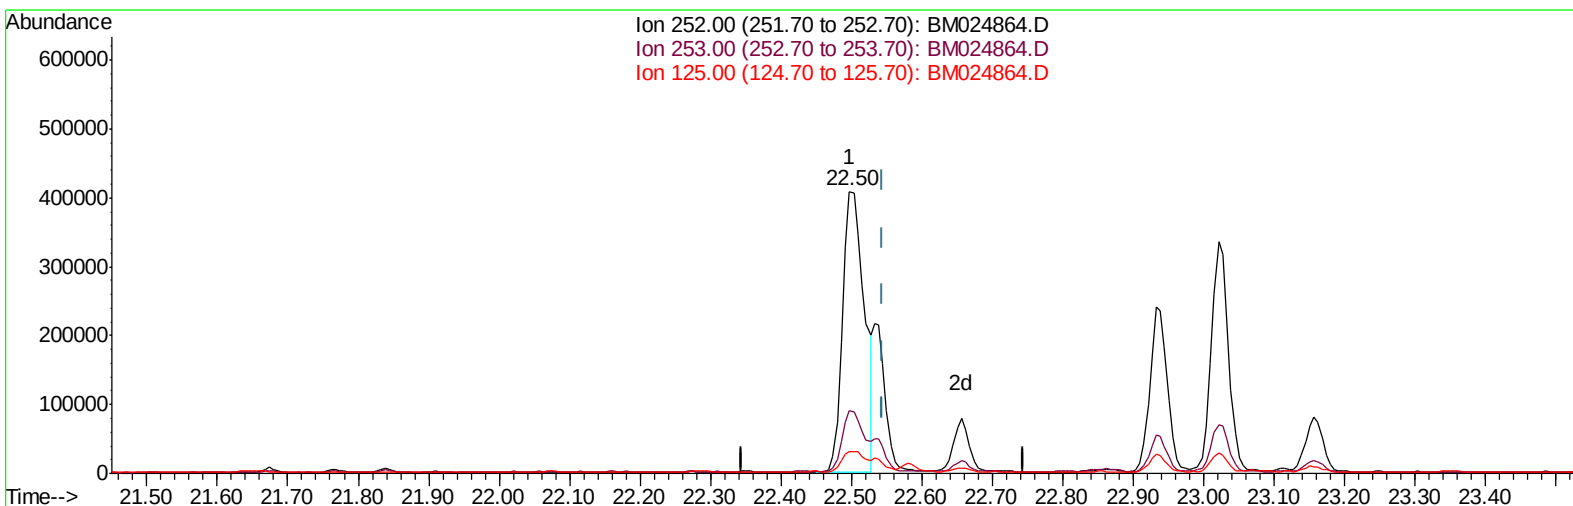

TIC: BM024864.D

(89) Benzo(k)fluoranthene
22.497min (-0.047) 6.75ng/ul
response 869187

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	22.25
125.00	6.40	7.85#
0.00	0.00	0.00