
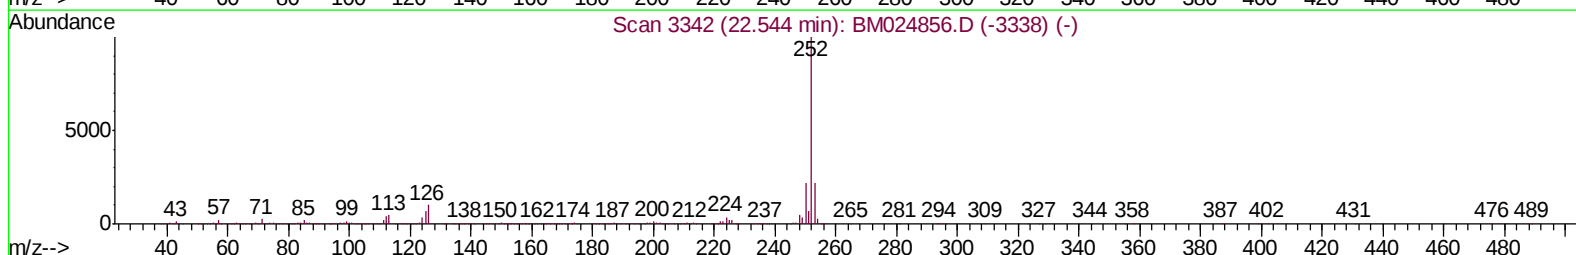
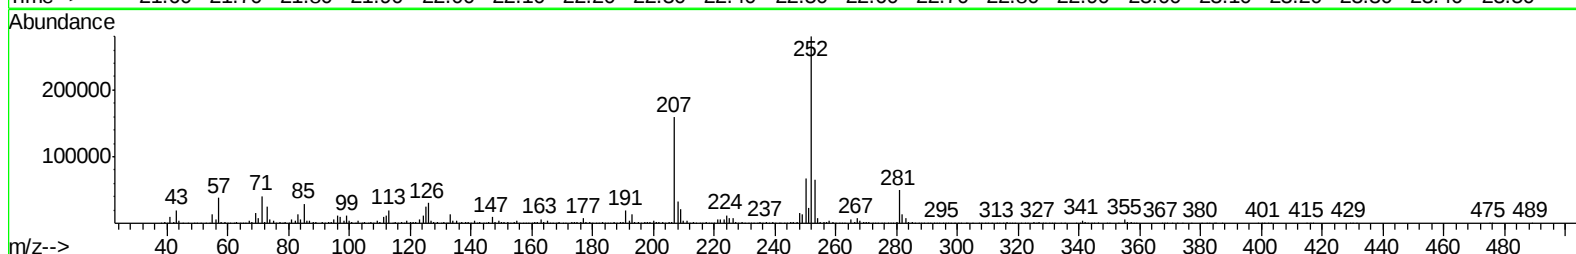


Data File : BM024865.D
Acq On : 13 Feb 2020 21:02
Operator : CG/JU
Sample : L1404-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Feb 14 06:03:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 14 05:59:53 2020
Response via : Initial Calibration

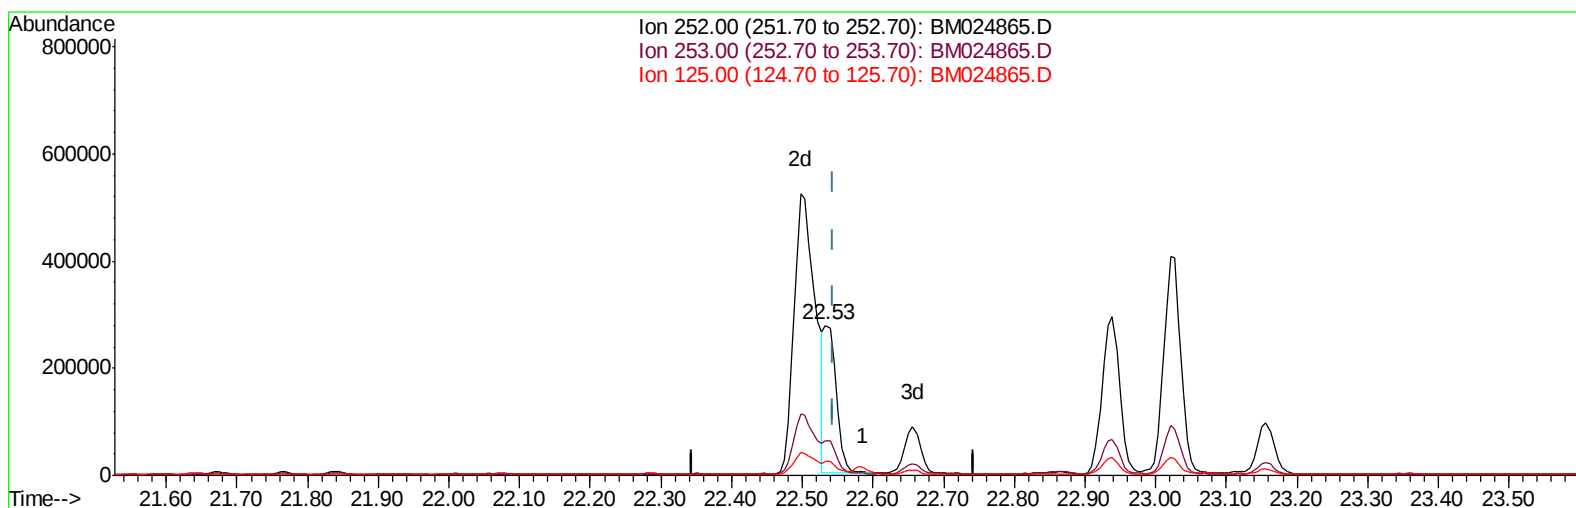

TIC: BM024865.D

(89) Benzo(k)fluoranthene

22.533min (-0.011) 2.61ng/ul m

response 327405

Ion	Exp%	Act%
252.00	100	100
253.00	21.70	23.20
125.00	6.40	9.29#
0.00	0.00	0.00