
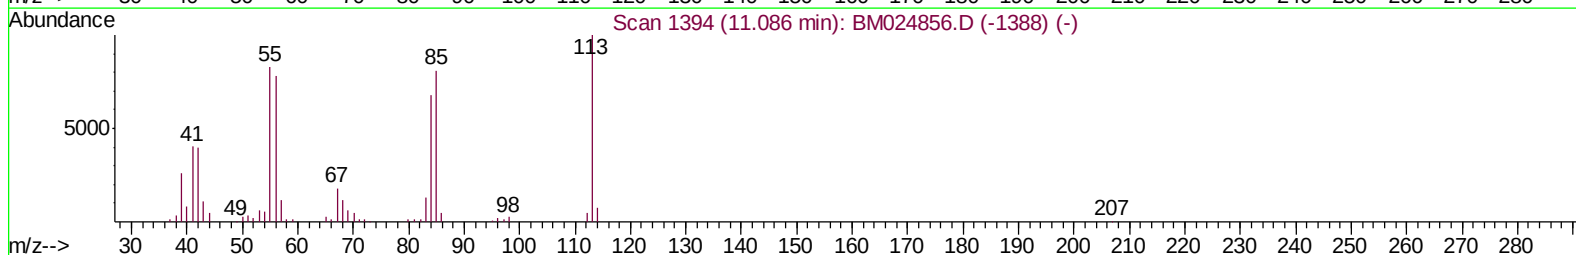
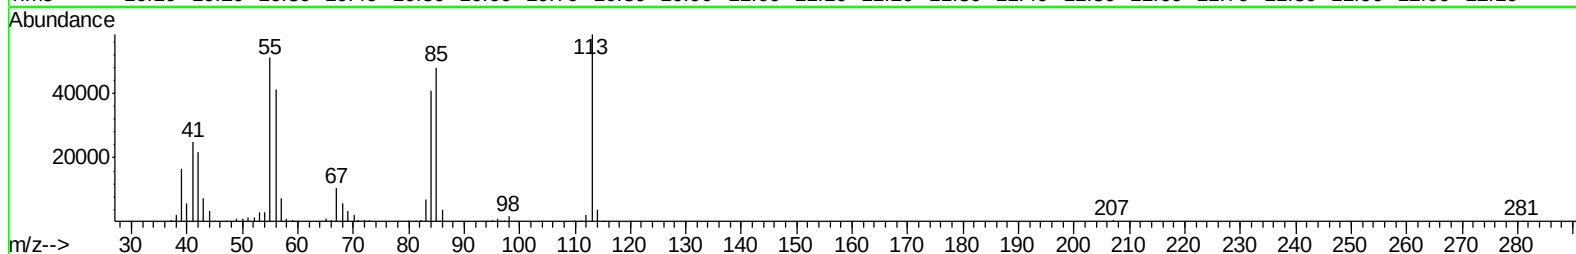


Data File : BM024872.D
Acq On : 14 Feb 2020 01:50
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Feb 14 06:04:28 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 14 05:59:53 2020
Response via : Initial Calibration

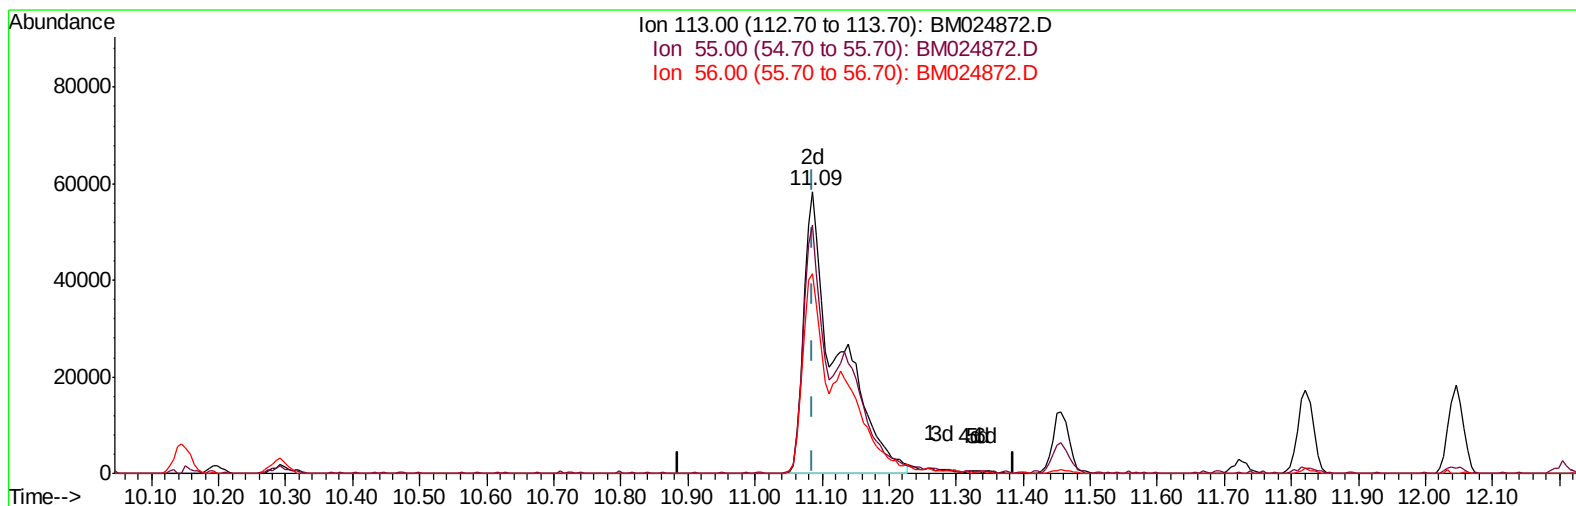

TIC: BM024872.D

(32) Caprolactam

11.086min (0.000) 33.97ng/ul m

response 201929

Ion	Exp%	Act%
113.00	100	100
55.00	107.70	88.04
56.00	89.90	70.71#
0.00	0.00	0.00