
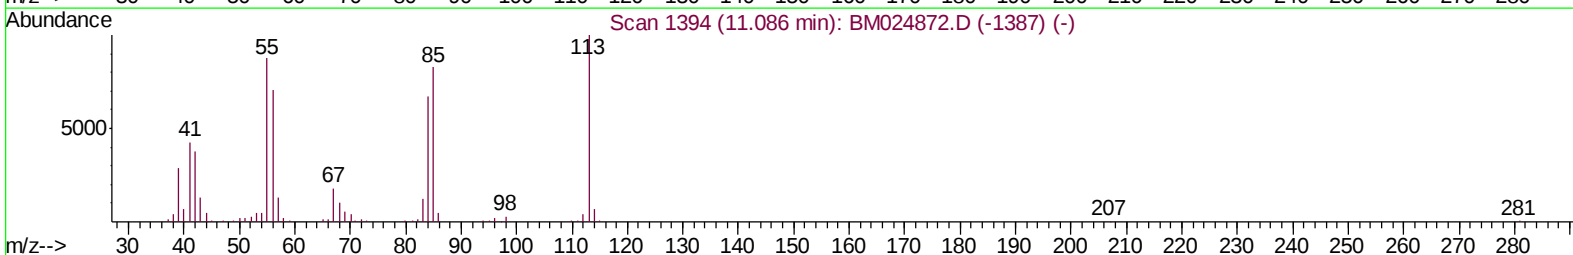
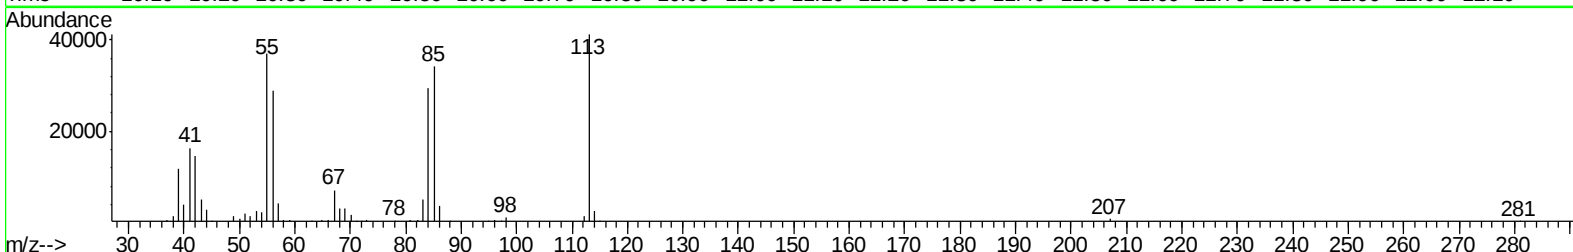


Data File : BM024879.D
Acq On : 14 Feb 2020 06:21
Operator : CG/JU
Sample : SSTDCCC020
Misc :
ALS Vial : 32 Sample Multiplier: 1

Quant Time: Feb 14 07:48:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 14 07:45:43 2020
Response via : Initial Calibration

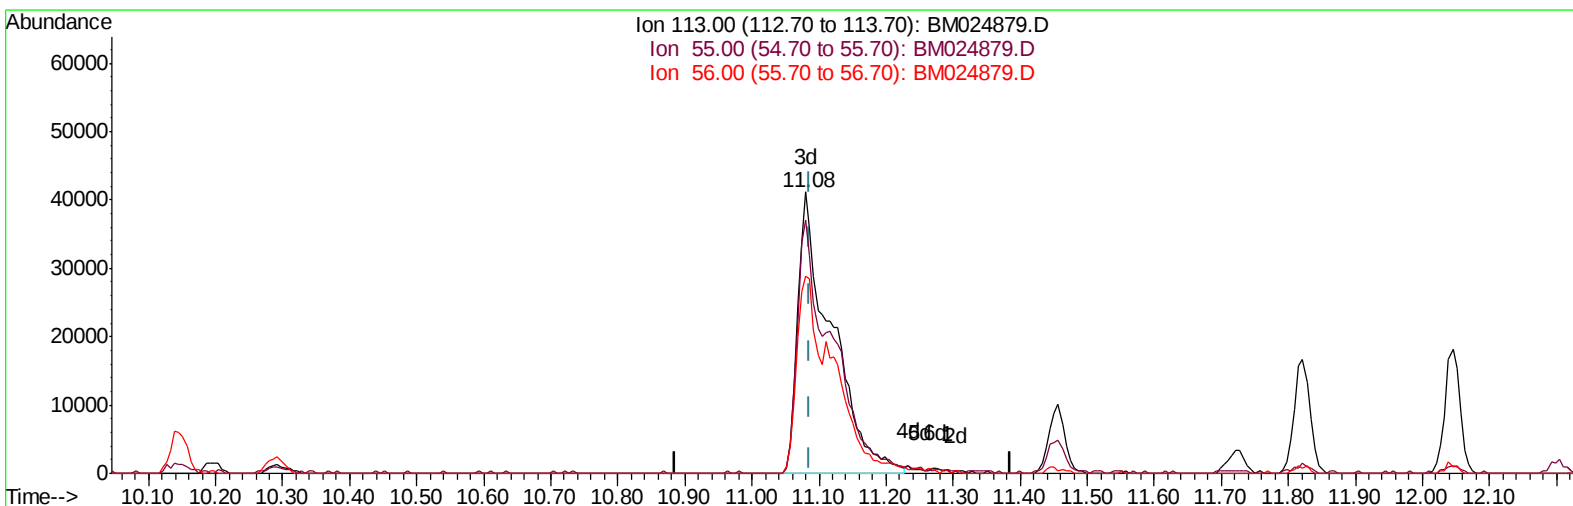

TIC: BM024879.D

(32) Caprolactam

11.080min (-0.006) 21.35ng/ul m

response 143509

Ion	Exp%	Act%
113.00	100	100
55.00	107.70	89.82
56.00	89.90	70.09#
0.00	0.00	0.00