
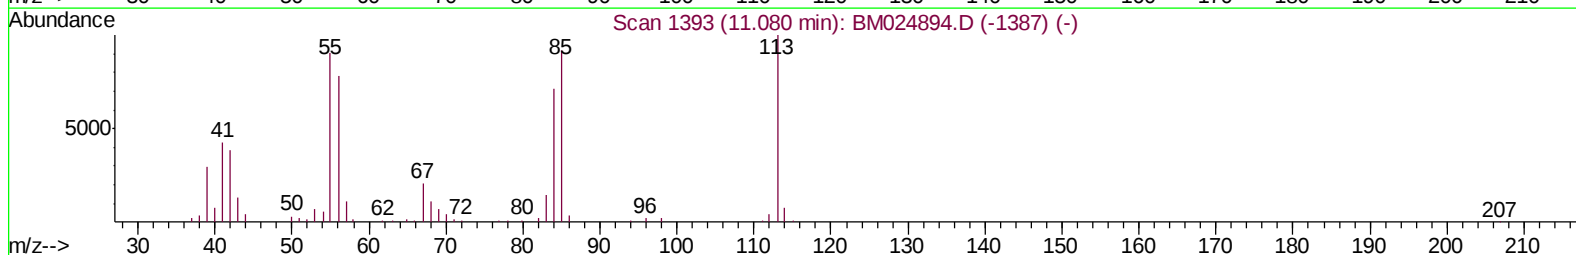
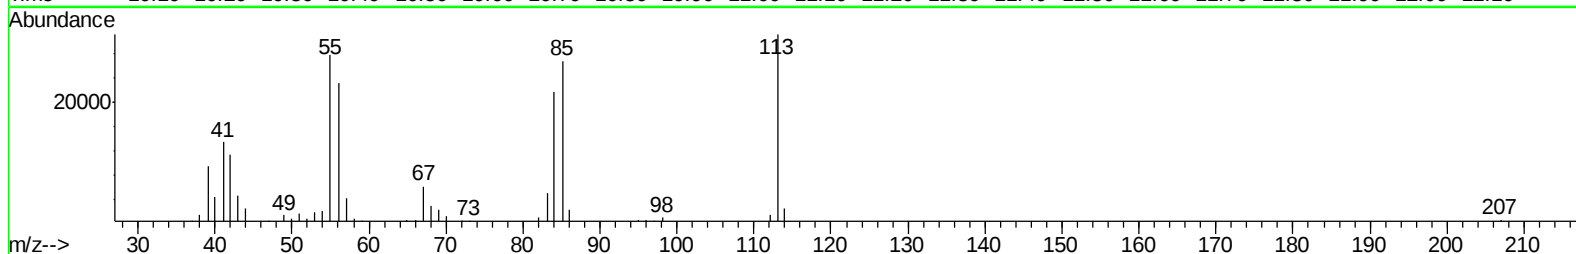


Data File : BM024902.D
Acq On : 14 Feb 2020 20:45
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 46 Sample Multiplier: 1

Quant Time: Feb 15 03:55:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 15 03:52:31 2020
Response via : Initial Calibration

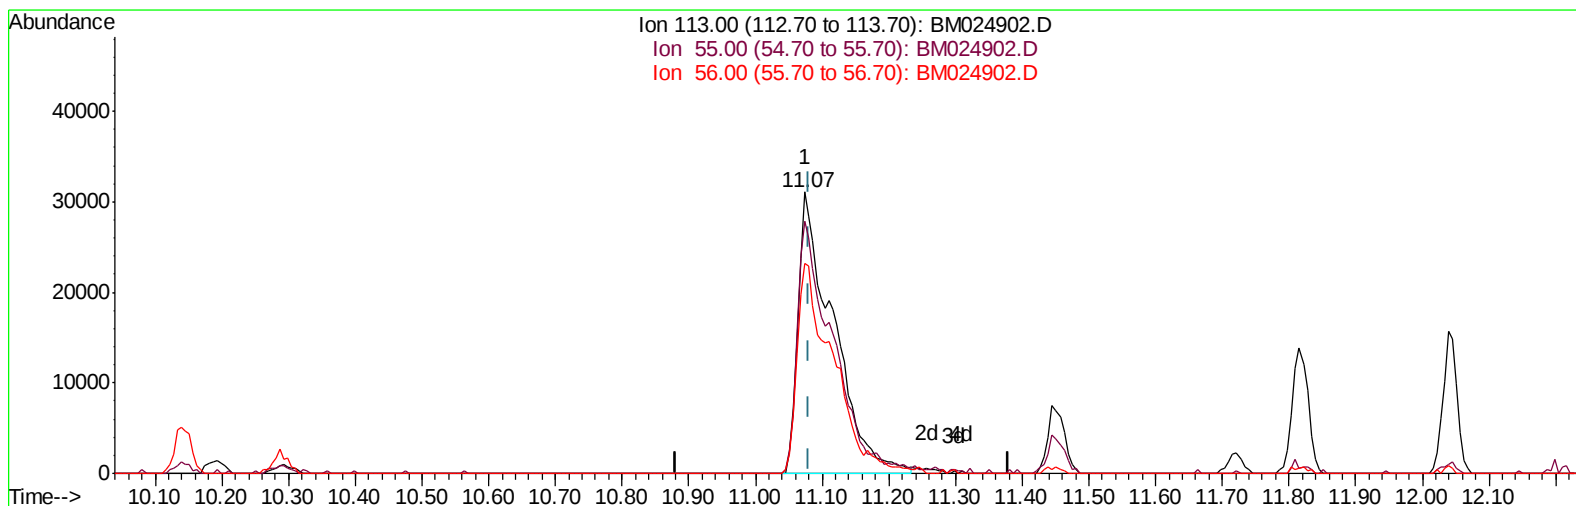

TIC: BM024902.D

(32) Caprolactam

11.075min (-0.006) 20.05ng/ul m

response 112456

Ion	Exp%	Act%
113.00	100	100
55.00	107.70	89.43
56.00	89.90	74.44
0.00	0.00	0.00