

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021320\
 Data File : BM024891.D
 Acq On : 14 Feb 2020 14:09
 Operator : CG/JU
 Sample : L1422-13
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C5AX6

Quant Time: Feb 14 15:38:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 14 07:45:43 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	357515	20.00	ng/ul	0.00
18) Naphthalene-d8	10.15	136	1302887	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.04	164	790188	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.80	188	1644833	20.00	ng/ul	0.00
78) Chrysene-d12	21.01	240	1638515	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	1742005	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	49565	6.67	ng/uL	0.00
5) Phenol-d5	6.59	99	812202	34.20	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.75	67	500603	37.32	ng/ul	0.00
9) 2-Chlorophenol-d4	6.93	132	695818	32.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	637780	31.82	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	336069	35.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.25	143	386753	34.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	696308	31.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	805357	38.34	ng/ul	0.00
44) Dimethylphthalate-d6	13.47	166	1986317	33.30	ng/ul	0.00
47) Acenaphthylene-d8	13.73	160	2471676	35.48	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	288571	29.77	ng/ul	0.00
58) Fluorene-d10	15.05	176	1763731	33.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.18	200	287801	26.84	ng/ul	0.00
71) Anthracene-d10	16.89	188	2612431	34.79	ng/ul	0.00
79) Pyrene-d10	19.20	212	2898447	35.36	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	3120166	35.66	ng/ul	0.00

Target Compounds


					Ovalue	
15) N-Nitroso-di-n-propylamine	8.10	70	16564	1.110	ng/ul#	1
45) Dimethylphthalate	13.52	163	218725	3.515	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021320\
Data File : BM024891.D
Acq On : 14 Feb 2020 14:09
Operator : CG/JU
Sample : L1422-13
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C5AX6

Quant Time: Feb 14 15:38:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 14 07:45:43 2020
Response via : Initial Calibration

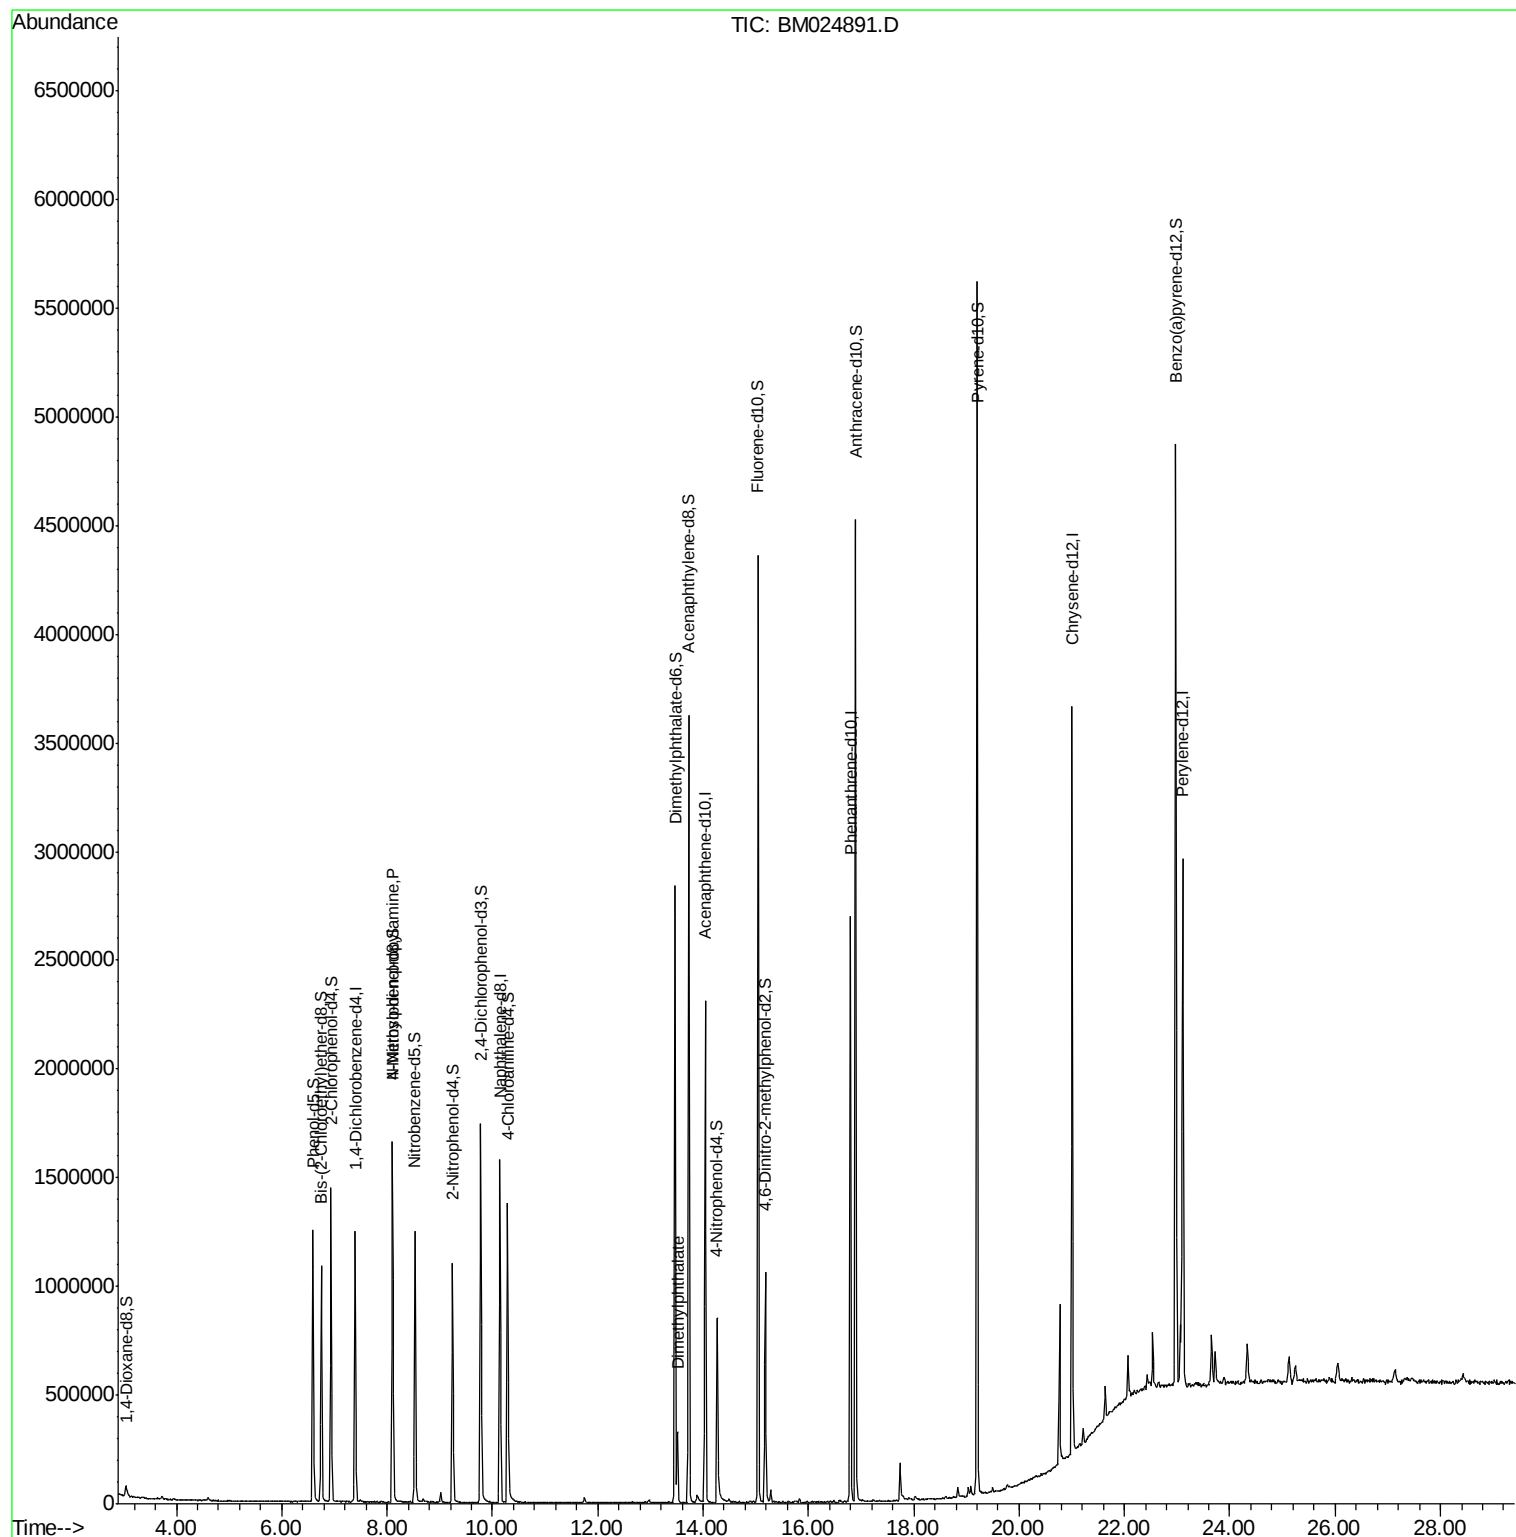

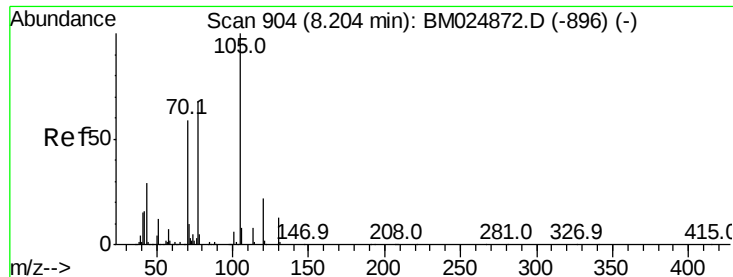

#15

N-Nitroso-di-n-propylamine

Concen: 1.110 ng/ul

RT: 8.10 min Scan# 887

Delta R.T. -0.10 min

Lab File: BM024891.D

Acq: 14 Feb 2020 14:09

Instrument :

BNA_M

ClientSampled :

C5AX6

Tot Ion: 70 Resp: 16564





Ion Ratio Lower Upper

70 100

42 189.3 35.6 53.4#

101 0.0 8.6 13.0#

130 0.0 18.6 28.0#

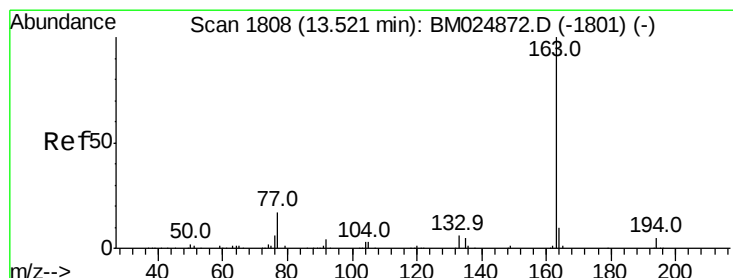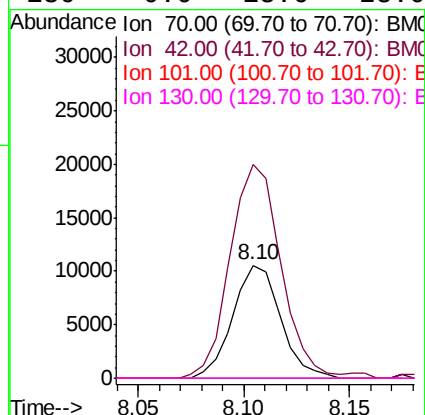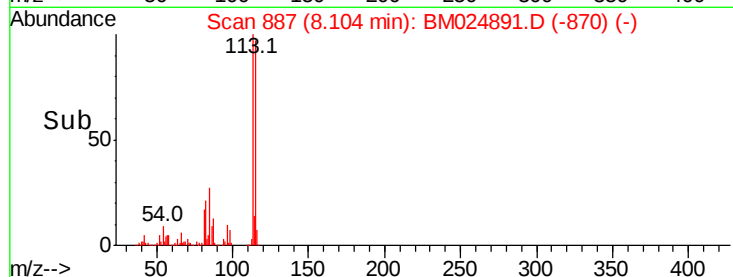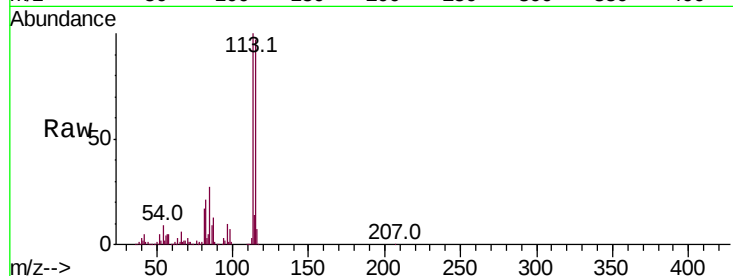

#45

Dimethylphthalate

Concen: 3.515 ng/ul

RT: 13.52 min Scan# 1807

Delta R.T. -0.01 min

Lab File: BM024891.D

Acq: 14 Feb 2020 14:09

Tgt Ion: 163 Resp: 218725

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 9.7 8.2 12.2

