

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021320\
 Data File : BM024867.D
 Acq On : 13 Feb 2020 22:15
 Operator : CG/JU
 Sample : L1404-10
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6N4

Manual Integrations
 APPROVED

mohammad
 2/17/2020 3:46:34 PM

Quant Time: Feb 14 06:51:48 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 14 05:59:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.40	152	435016	20.00	ng/ul	0.00
18) Naphthalene-d8	10.15	136	1584259	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.05	164	954661	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.80	188	1949432	20.00	ng/ul	0.00
78) Chrysene-d12	21.01	240	1885333	20.00	ng/ul	0.00
86) Perylene-d12	23.11	264	2017915	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.03	96	34478	3.81	ng/uL	0.00
5) Phenol-d5	6.60	99	591437	20.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.75	67	354570	21.72	ng/ul	0.00
9) 2-Chlorophenol-d4	6.94	132	497462	19.21	ng/ul	0.00
13) 4-Methylphenol-d8	8.11	113	314003	12.88	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	236237	20.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.25	143	280776	20.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	474943	17.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	360329	14.11	ng/ul	0.00
44) Dimethylphthalate-d6	13.47	166	1457424	20.22	ng/ul	0.00
47) Acenaphthylene-d8	13.73	160	1739203	20.67	ng/ul	0.00
52) 4-Nitrophenol-d4	14.27	143	193509	16.53	ng/ul	0.00
58) Fluorene-d10	15.05	176	1258940	19.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.18	200	208849	16.44	ng/ul	0.00
71) Anthracene-d10	16.90	188	1685405	18.94	ng/ul	0.00
79) Pyrene-d10	19.20	212	2071342	21.96	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.98	264	2138769	21.10	ng/ul	0.00

Target Compounds

					Ovalue	
70) Phenanthrene	16.84	178	1063275	10.003	ng/ul	98
72) Anthracene	16.93	178	173495	1.609	ng/ul	99
77) Fluoranthene	18.87	202	1604431	12.296	ng/ul#	96
80) Pyrene	19.23	202	1475965	11.827	ng/ul#	95
83) Benzo(a)anthracene	21.00	228	790086	6.221	ng/ul	98
85) Chrysene	21.05	228	819341	6.553	ng/ul	99
88) Benzo(b)fluoranthene	22.50	252	1040276	8.107	ng/ul#	97
89) Benzo(k)fluoranthene	22.53	252	402991m	3.263	ng/ul	
91) Benzo(a)pyrene	23.02	252	709106	6.164	ng/ul#	98
92) Indeno(1,2,3-cd)pyrene	25.16	276	553793	3.867	ng/ul	99
93) Dibenzo(a,h)anthracene	25.17	278	149189	1.223	ng/ul#	91
94) Benzo(g,h,i)perylene	25.77	276	488198	4.099	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021320\
Data File : BM024867.D
Acq On : 13 Feb 2020 22:15
Operator : CG/JU
Sample : L1404-10
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
CB6N4

Quant Time: Feb 14 06:51:48 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 14 05:59:53 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
2/17/2020 3:46:34 PM

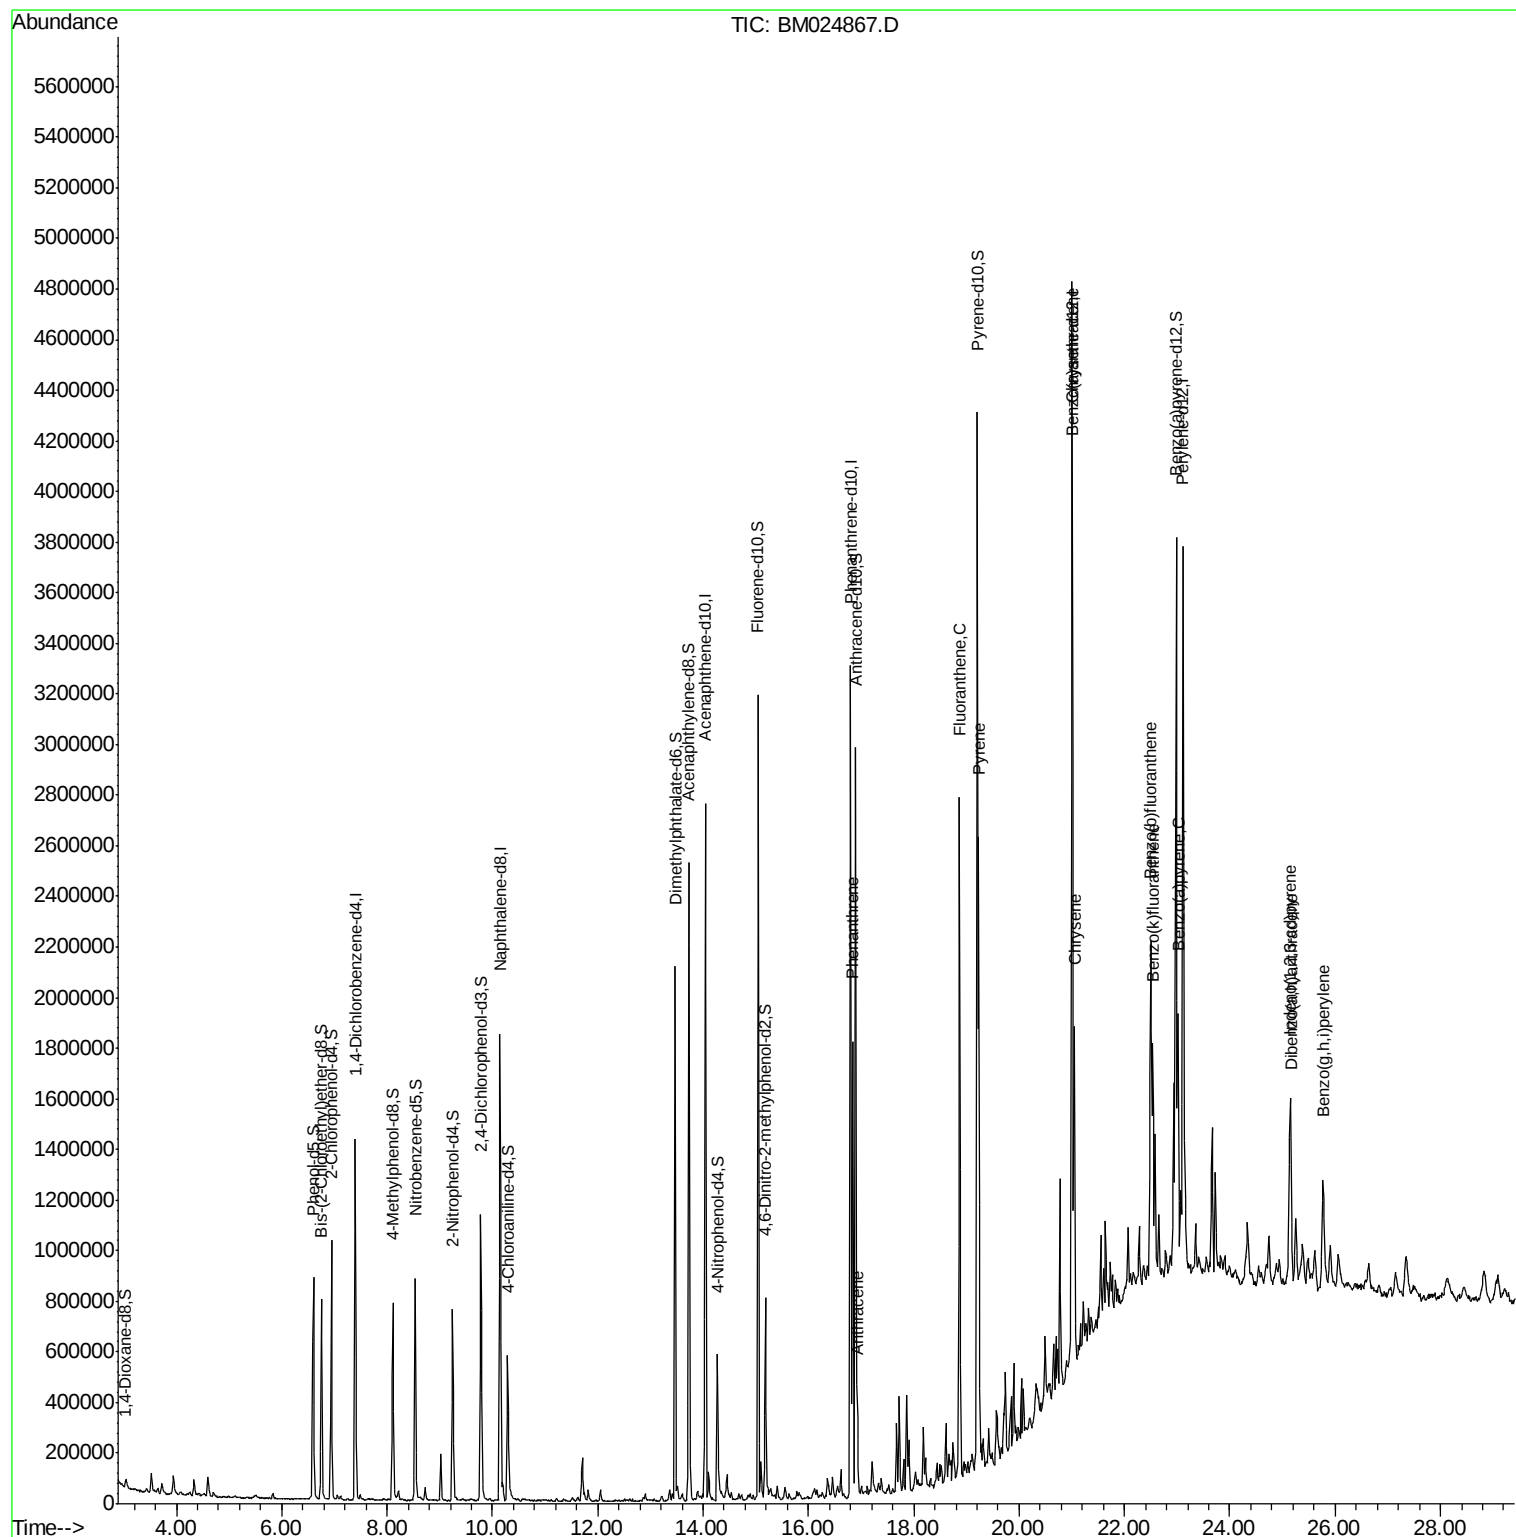

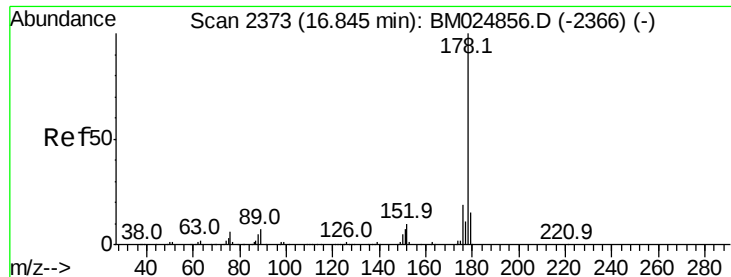

#70

Phenanthrene

Concen: 10.003 ng/ul

RT: 16.84 min Scan# 2372

Delta R.T. -0.01 min

Lab File: BM024867.D

Acq: 13 Feb 2020 22:15

Instrument :

BNA_M

ClientSampled :

CB6N4

Tot Ion:178 Resp: 1063275

Ion Ratio Lower Upper

178 100

179 15.7 12.2 18.2


176 19.1 14.5 21.7

Manual Integrations

APPROVED

mohammad




2/17/2020 3:46:34 PM

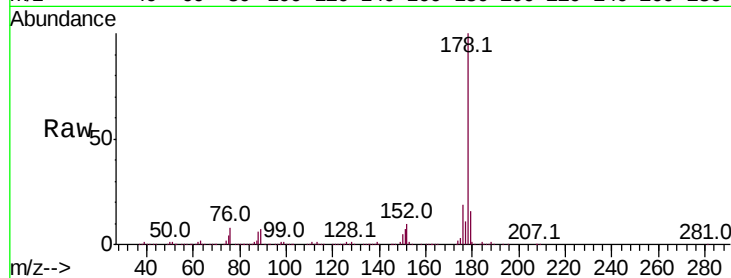

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

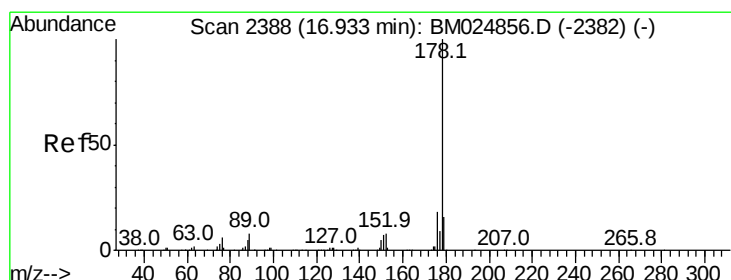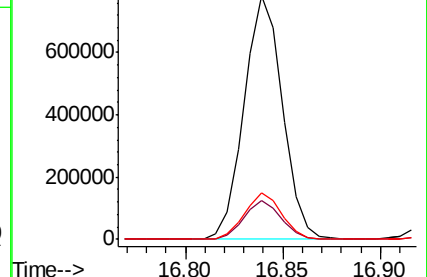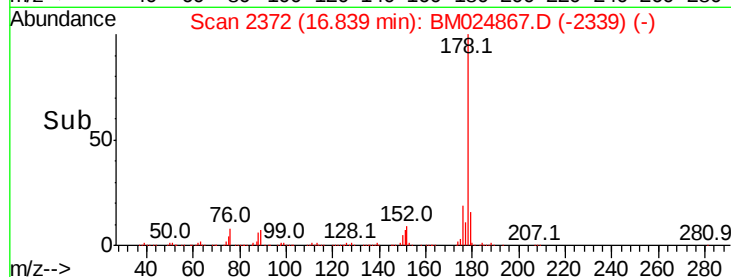

#72

Anthracene

Concen: 1.609 ng/ul

RT: 16.93 min Scan# 2388

Delta R.T. 0.00 min

Lab File: BM024867.D

Acq: 13 Feb 2020 22:15


Tgt Ion:178 Resp: 173495

Ion Ratio Lower Upper

178 100

179 16.1 12.3 18.5



176 17.5 14.1 21.1

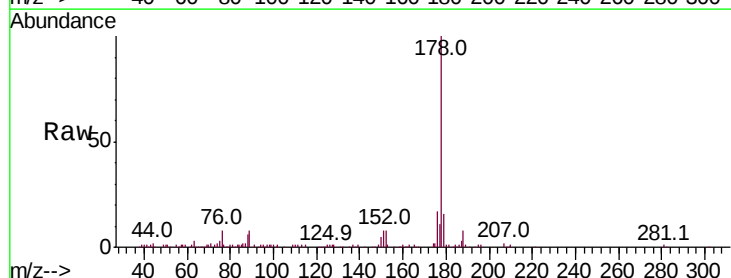


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

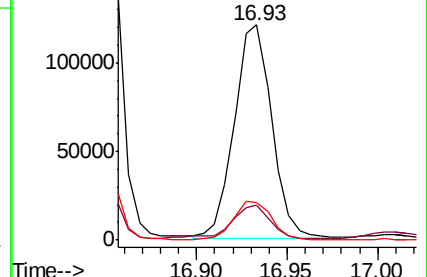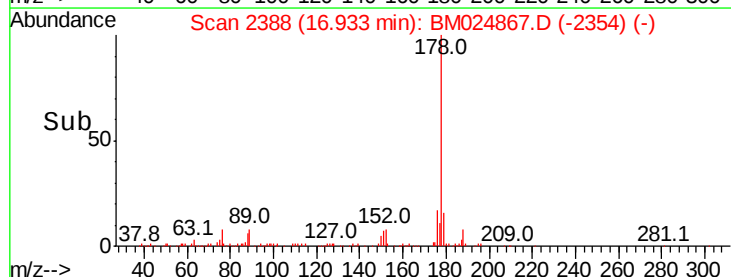

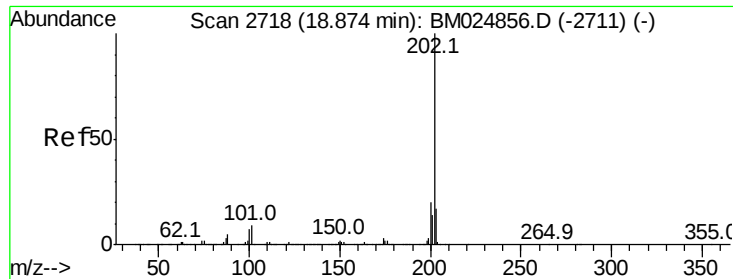

#77

Fluoranthene

Concen: 12.296 ng/ul

RT: 18.87 min Scan# 2717

Delta R.T. -0.01 min

Lab File: BM024867.D

Acq: 13 Feb 2020 22:15

Instrument :

BNA_M





ClientSampleId :

CB6N4

Tot Ion:	202	Resp:	1604431
Ion Ratio	Lower	Upper	
202	100		
101	9.3	6.1	9.1#
100	7.2	4.8	7.2#

Manual Integrations
APPROVED

mohammad
2/17/2020 3:46:34 PM

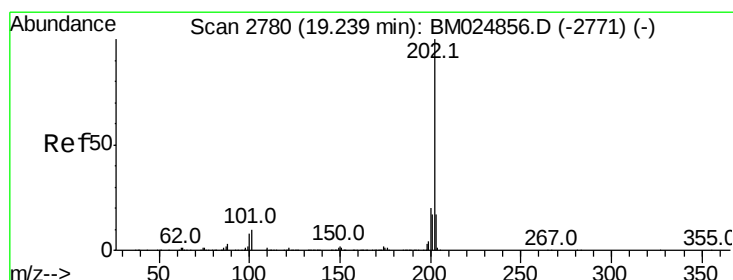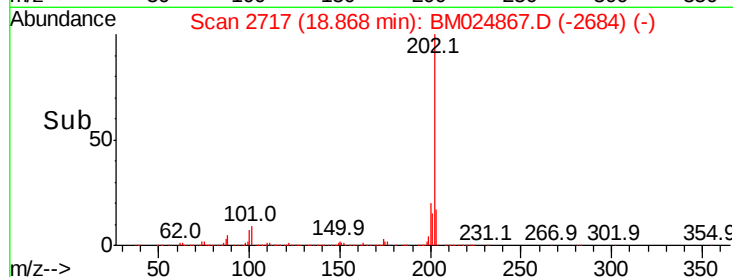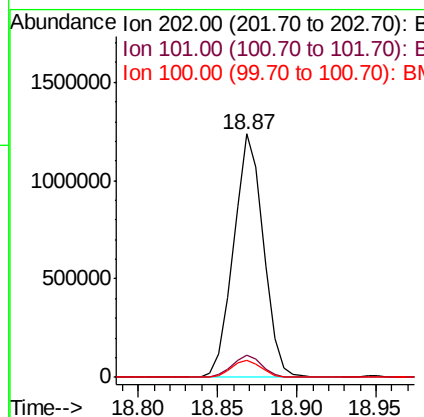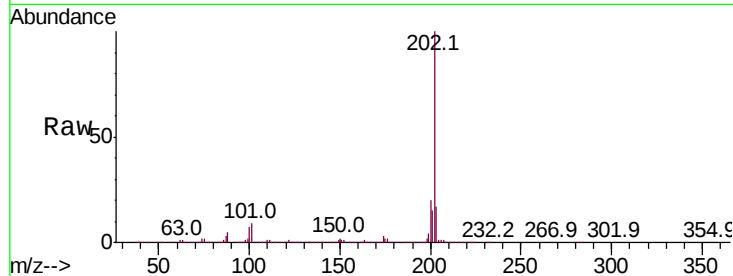

#80

Pyrene

Concen: 11.827 ng/ul




RT: 19.23 min Scan# 2779


Delta R.T. -0.01 min

Lab File: BM024867.D

Acq: 13 Feb 2020 22:15

Tgt Ion:	202	Resp:	1475965
Ion Ratio	Lower	Upper	
202	100		
101	10.9	7.0	10.4#
100	8.9	5.8	8.8#

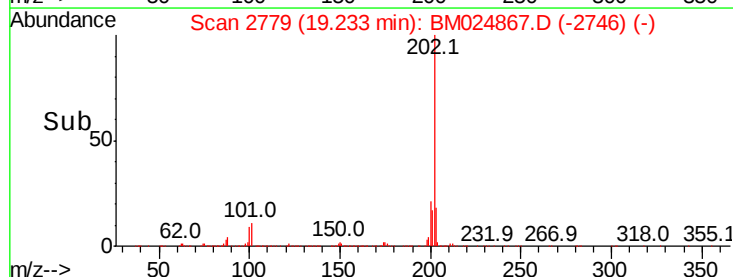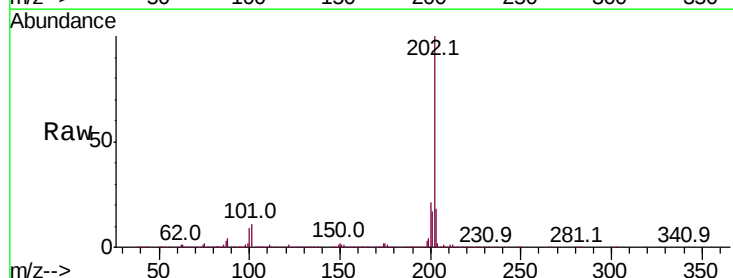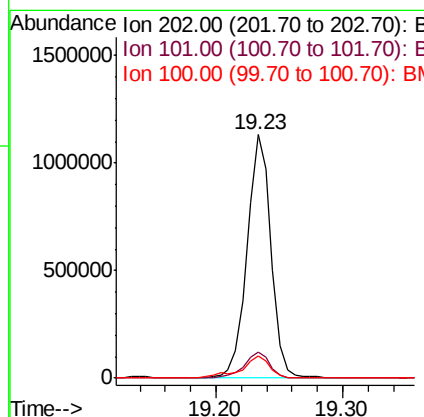

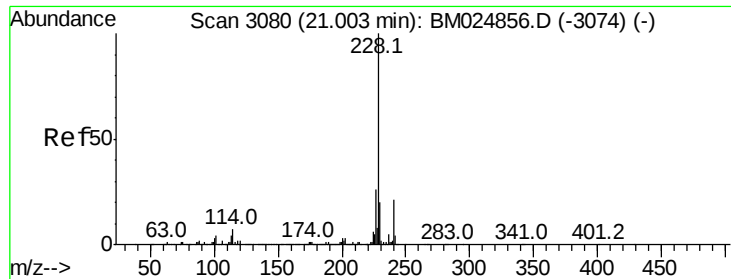





#83
Benzo(a)anthracene
Concen: 6.221 ng/ul
RT: 21.00 min Scan# 3079
Delta R.T. -0.01 min
Lab File: BM024867.D
Acq: 13 Feb 2020 22:15

Instrument :
BNA_M
ClientSampleId :
CB6N4

Tot Ion	Ratio	Lower	Upper
228	100		
229	20.0	15.9	23.9
226	27.6	20.8	31.2




Manual Integrations
APPROVED


mohammad
2/17/2020 3:46:34 PM

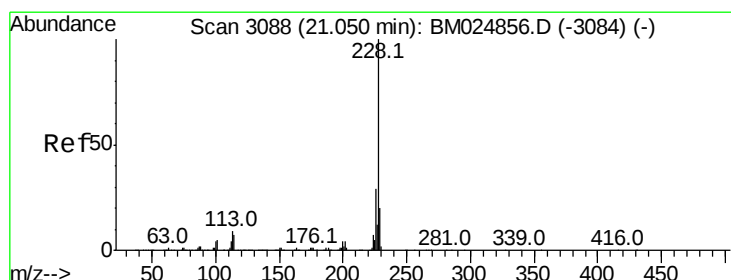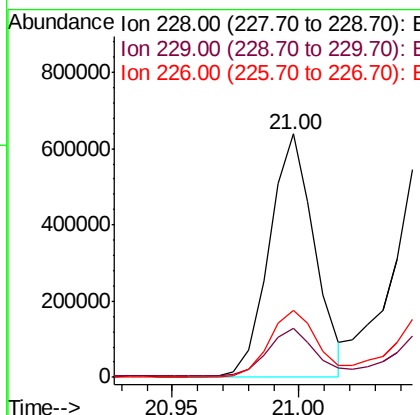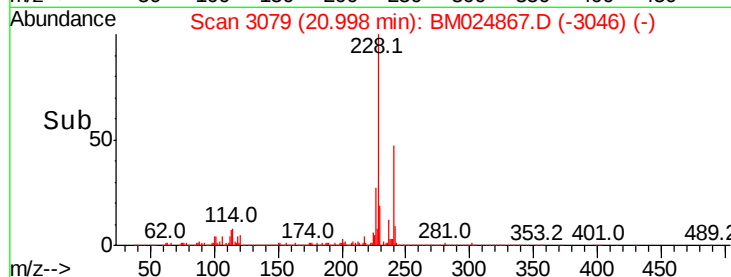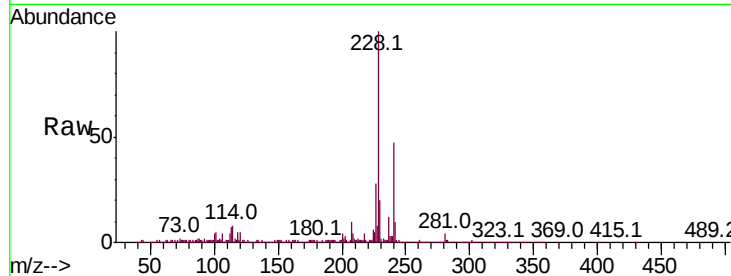

#85
Chrysene
Concen: 6.553 ng/ul
RT: 21.05 min Scan# 3088
Delta R.T. 0.00 min
Lab File: BM024867.D
Acq: 13 Feb 2020 22:15

Tgt Ion	Ratio	Lower	Upper
228	100		
226	27.9	23.0	34.4
229	20.3	15.8	23.8

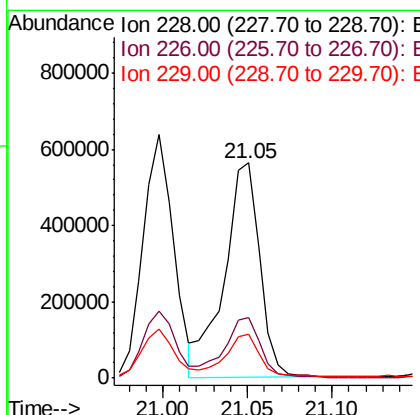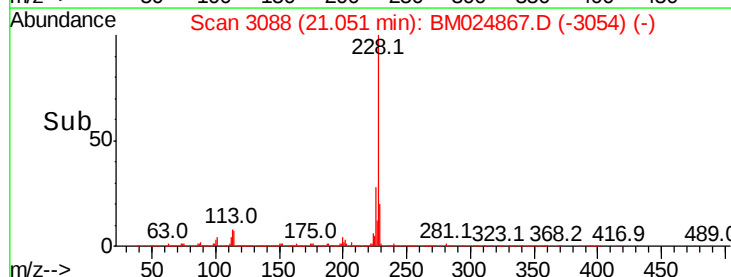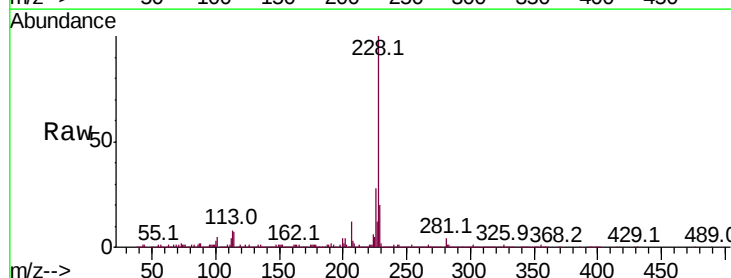

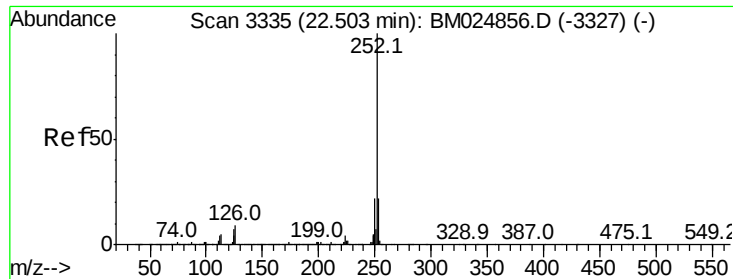

#88

Benzo(b)fluoranthene

Concen: 8.107 ng/ul

RT: 22.50 min Scan# 3334

Delta R.T. -0.01 min

Lab File: BM024867.D





Acq: 13 Feb 2020 22:15

Instrument :
BNA_M
ClientSampleId :
CB6N4

Tot Ion	Ratio	Lower	Upper
252	100		
253	22.7	17.3	25.9
125	8.0	5.1	7.7#

Manual Integrations
APPROVED

mohammad
2/17/2020 3:46:34 PM

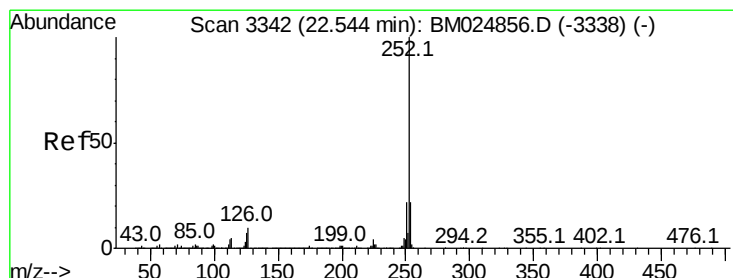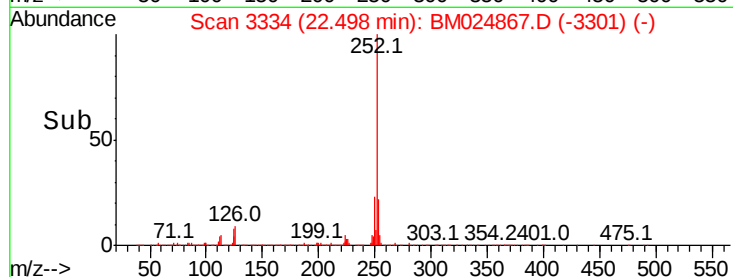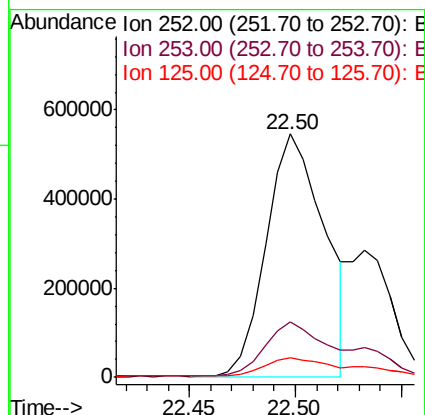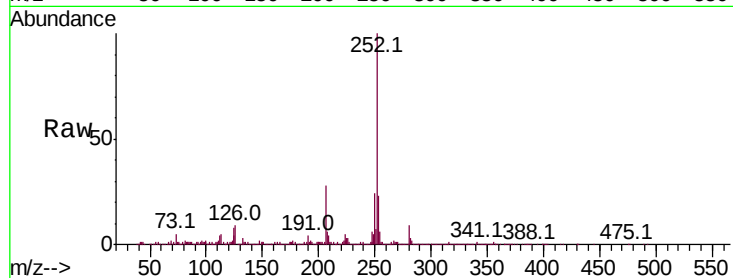

#89

Benzo(k)fluoranthene

Concen: 3.263 ng/ul m




RT: 22.53 min Scan# 3340


Delta R.T. -0.01 min

Lab File: BM024867.D

Acq: 13 Feb 2020 22:15

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.4	26.0
125	8.4	5.1	7.7#

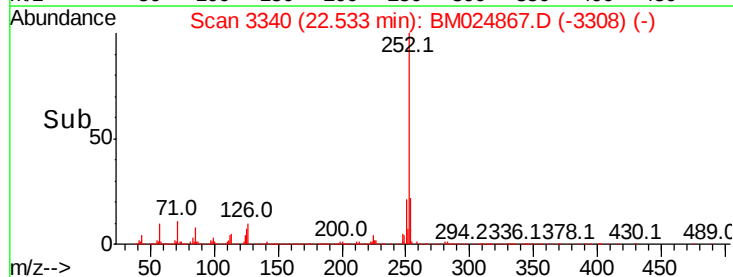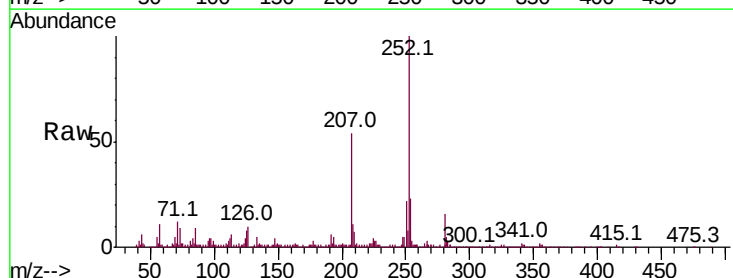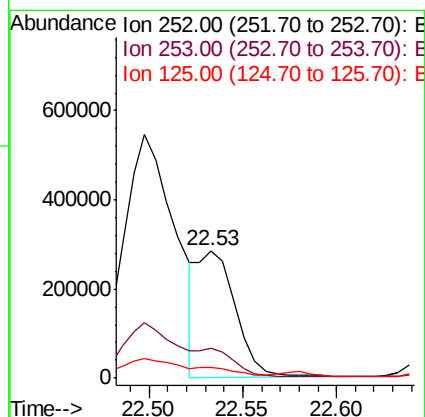

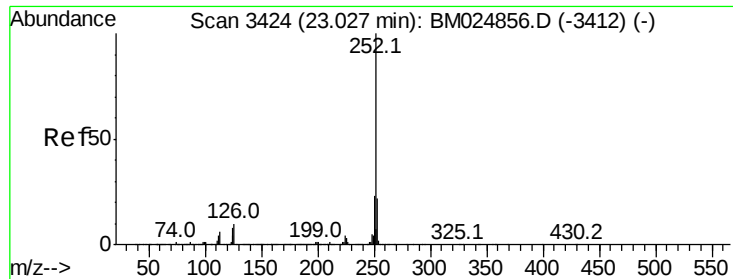





#91
Benzo(a)pyrene
Concen: 6.164 ng/u1
RT: 23.02 min Scan# 3423
Delta R.T. -0.01 min
Lab File: BM024867.D
Acq: 13 Feb 2020 22:15

Instrument :
BNA_M
ClientSampleId :
CB6N4

Tot Ion:	252	Resp:	709106
Ion Ratio	Lower	Upper	
252	100		
253	22.3	17.5	26.3
125	8.6	5.6	8.4




Manual Integrations
APPROVED


mohammad
2/17/2020 3:46:34 PM

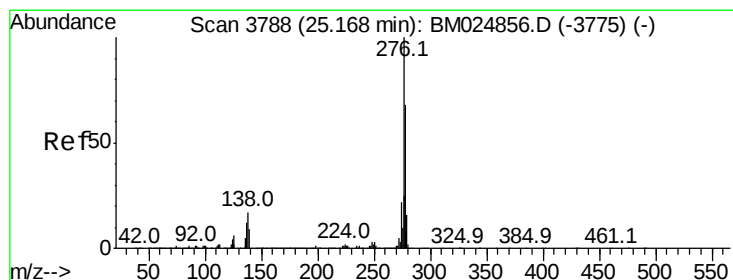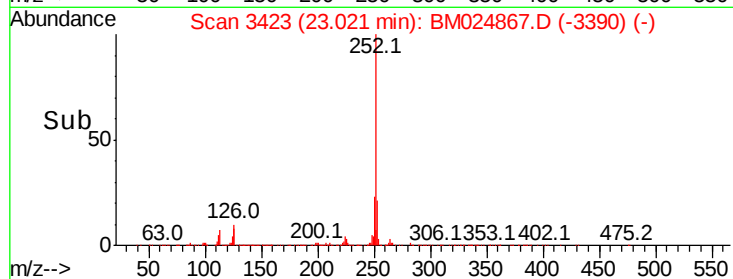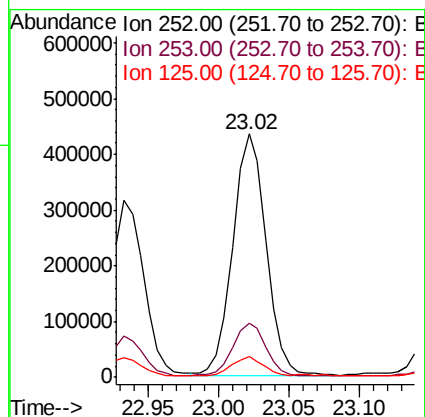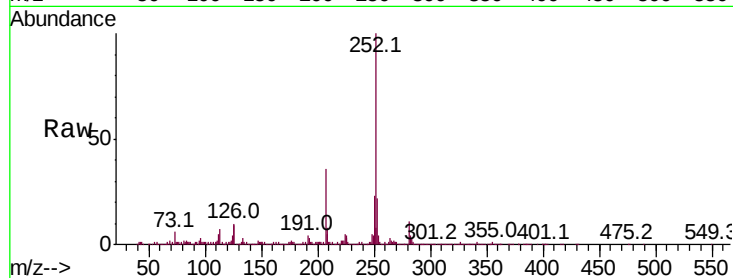

#92
Indeno(1,2,3-cd)pyrene
Concen: 3.867 ng/u1
RT: 25.16 min Scan# 3786
Delta R.T. -0.01 min
Lab File: BM024867.D
Acq: 13 Feb 2020 22:15

Tgt Ion:	276	Resp:	553793
Ion Ratio	Lower	Upper	
276	100		
138	15.4	12.8	19.2
277	24.6	19.3	28.9

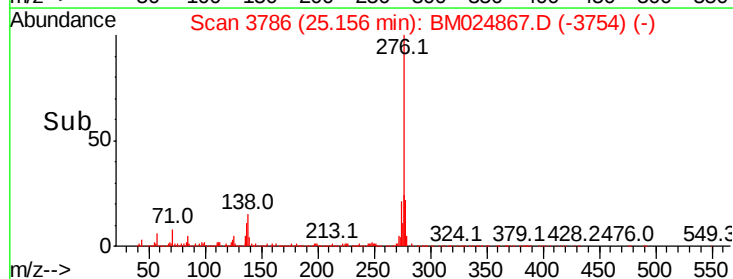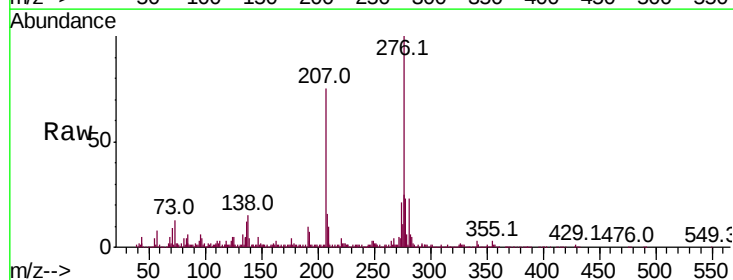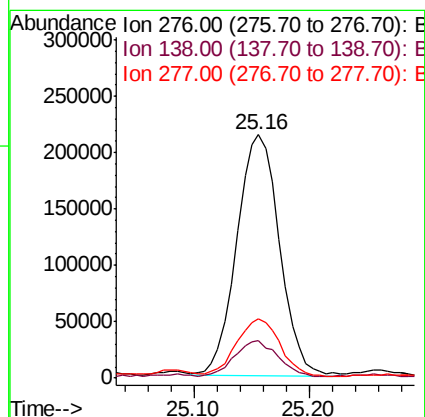

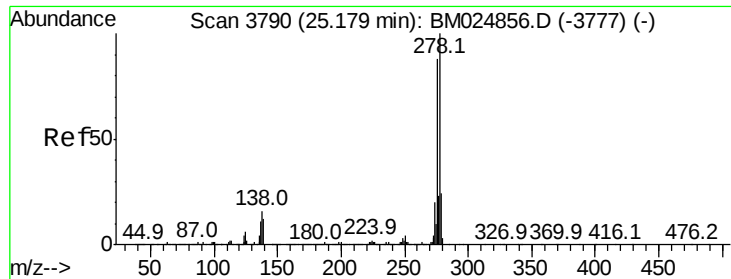


#93
Dibenzo(a,h)anthracene
Concen: 1.223 ng/ul
RT: 25.17 min Scan# 3788
Delta R.T. -0.01 min
Lab File: BM024867.D
Acq: 13 Feb 2020 22:15

Instrument :
BNA_M
ClientSampleId :
CB6N4




Tot Ion	Ratio	Lower	Upper
278	100		
139	0.0	8.4	12.6#
279	22.7	18.5	27.7

Manual Integrations
APPROVED

mohammad
2/17/2020 3:46:34 PM

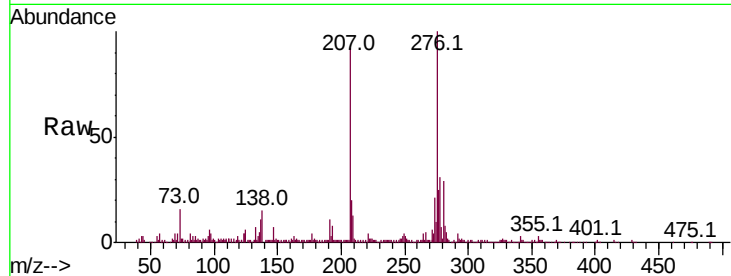

Abundance Ion 278.00 (277.70 to 278.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 279.00 (278.70 to 279.70): E

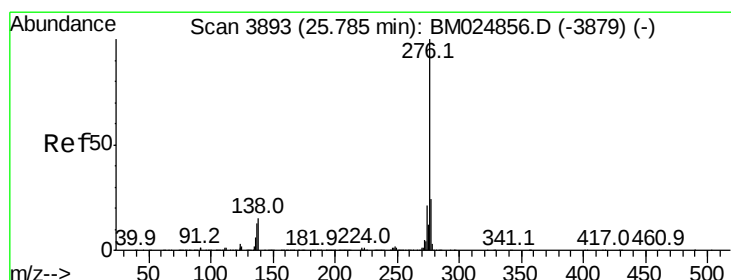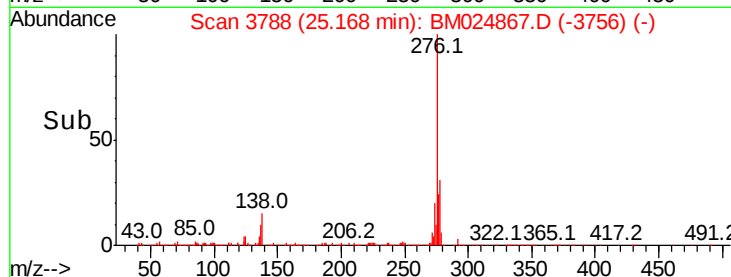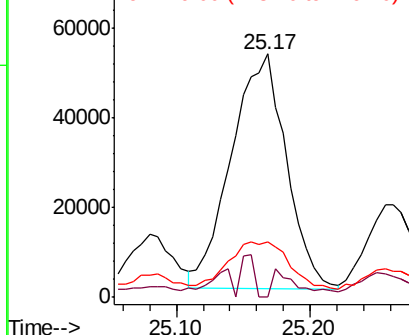

#94
Benzo(g,h,i)perylene
Concen: 4.099 ng/ul
RT: 25.77 min Scan# 3891
Delta R.T. -0.01 min
Lab File: BM024867.D
Acq: 13 Feb 2020 22:15

Tgt Ion	Ratio	Lower	Upper
276	100		
138	15.2	11.8	17.6
277	25.1	19.0	28.6

Abundance Ion 276.00 (275.70 to 276.70): E
Ion 138.00 (137.70 to 138.70): E
Ion 277.00 (276.70 to 277.70): E

