

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021320\
 Data File : BM024878.D
 Acq On : 14 Feb 2020 05:45
 Operator : CG/JU
 Sample : L1404-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6Y0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.040	21	26	36	rVB	40122	94400	1.91%	0.158%
2	3.716	138	141	148	rVV3	10362	21173	0.43%	0.035%
3	6.593	622	630	642	rBV	894921	1498925	30.28%	2.503%
4	6.751	651	657	667	rBV	786680	1251918	25.29%	2.090%
5	6.934	682	688	698	rBV	1039850	1739664	35.14%	2.905%
6	7.393	759	766	778	rBV	1230974	1967095	39.74%	3.284%
7	8.104	880	887	899	rBV	1142776	1900817	38.40%	3.174%
8	8.534	952	960	970	rBV	860411	1453940	29.37%	2.428%
9	9.022	1039	1043	1050	rVB4	12393	20017	0.40%	0.033%
10	9.245	1074	1081	1091	rBV	761025	1240868	25.07%	2.072%
11	9.781	1165	1172	1186	rBV	1209137	2072621	41.87%	3.461%
12	9.881	1188	1189	1193	rVB2	5134	5416	0.11%	0.009%
13	10.145	1227	1234	1243	rBV	1598130	2569494	51.90%	4.290%
14	10.292	1251	1259	1278	rBV	957257	1845713	37.28%	3.082%
15	11.751	1501	1507	1512	rBV2	18938	29186	0.59%	0.049%
16	12.963	1707	1713	1718	rBV3	16117	26885	0.54%	0.045%
17	13.351	1774	1779	1783	rVB5	4543	6769	0.14%	0.011%
18	13.469	1792	1799	1804	rBV	1926990	2639752	53.32%	4.407%
19	13.516	1804	1807	1819	rVB	44527	74398	1.50%	0.124%
20	13.727	1836	1843	1852	rBV	2353631	3472349	70.14%	5.798%
21	13.886	1865	1870	1879	rBV2	37597	84047	1.70%	0.140%
22	14.039	1890	1896	1906	rVB	2231993	3375235	68.18%	5.635%
23	14.269	1929	1935	1955	rBV	524649	1032877	20.86%	1.725%
24	14.892	2035	2041	2046	rBV8	5578	7656	0.15%	0.013%
25	15.045	2060	2067	2078	rBV	3019098	4174385	84.32%	6.970%
26	15.180	2084	2090	2103	rBV	697913	1038819	20.98%	1.734%
27	15.286	2103	2108	2114	rVB2	36857	53578	1.08%	0.089%
28	15.833	2195	2201	2206	rBV6	9593	19807	0.40%	0.033%
29	15.998	2228	2229	2236	rVB4	5166	8144	0.16%	0.014%
30	16.074	2236	2242	2244	rBV6	4873	9432	0.19%	0.016%
31	16.480	2309	2311	2315	rBV4	5160	6402	0.13%	0.011%
32	16.580	2325	2328	2332	rBV	9972	11679	0.24%	0.019%
33	16.798	2358	2365	2375	rBV	2833017	3795587	76.67%	6.337%
34	16.898	2375	2382	2393	rVV	2871098	4211702	85.08%	7.032%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021320\
 Data File : BM024878.D
 Acq On : 14 Feb 2020 05:45
 Operator : CG/JU
 Sample : L1404-20
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB6Y0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
 Title : SVOA CALIBRATION

35	17.227	2435	2438	2441	rBV3	11243	11659	0.24%	0.019%
36	17.739	2522	2525	2531	rBV7	14616	26459	0.53%	0.044%
37	17.862	2545	2546	2550	rVB4	6614	6148	0.12%	0.010%
38	18.027	2570	2574	2576	rBV5	4909	7584	0.15%	0.013%
39	18.186	2597	2601	2604	rBV6	10484	12801	0.26%	0.021%
40	18.610	2670	2673	2678	rVB6	12045	15483	0.31%	0.026%
41	18.839	2708	2712	2718	rBV	36765	44129	0.89%	0.074%
42	19.092	2751	2755	2761	rVB	27707	40577	0.82%	0.068%
43	19.204	2768	2774	2783	rBV	3659480	4950495	100.00%	8.266%
44	19.274	2783	2786	2790	rVV6	22783	32073	0.65%	0.054%
45	20.768	3036	3040	3045	rBV3	130587	206848	4.18%	0.345%
46	21.009	3076	3081	3091	rBV	3219248	4061853	82.05%	6.782%
47	22.980	3409	3416	3425	rBV	2737107	4638322	93.69%	7.744%
48	23.109	3432	3438	3446	rVB	2314758	4077898	82.37%	6.809%


Sum of corrected areas: 59893079

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM021320\
Data File : BM024878.D
Acq On : 14 Feb 2020 05:45
Operator : CG/JU
Sample : L1404-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB6Y0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

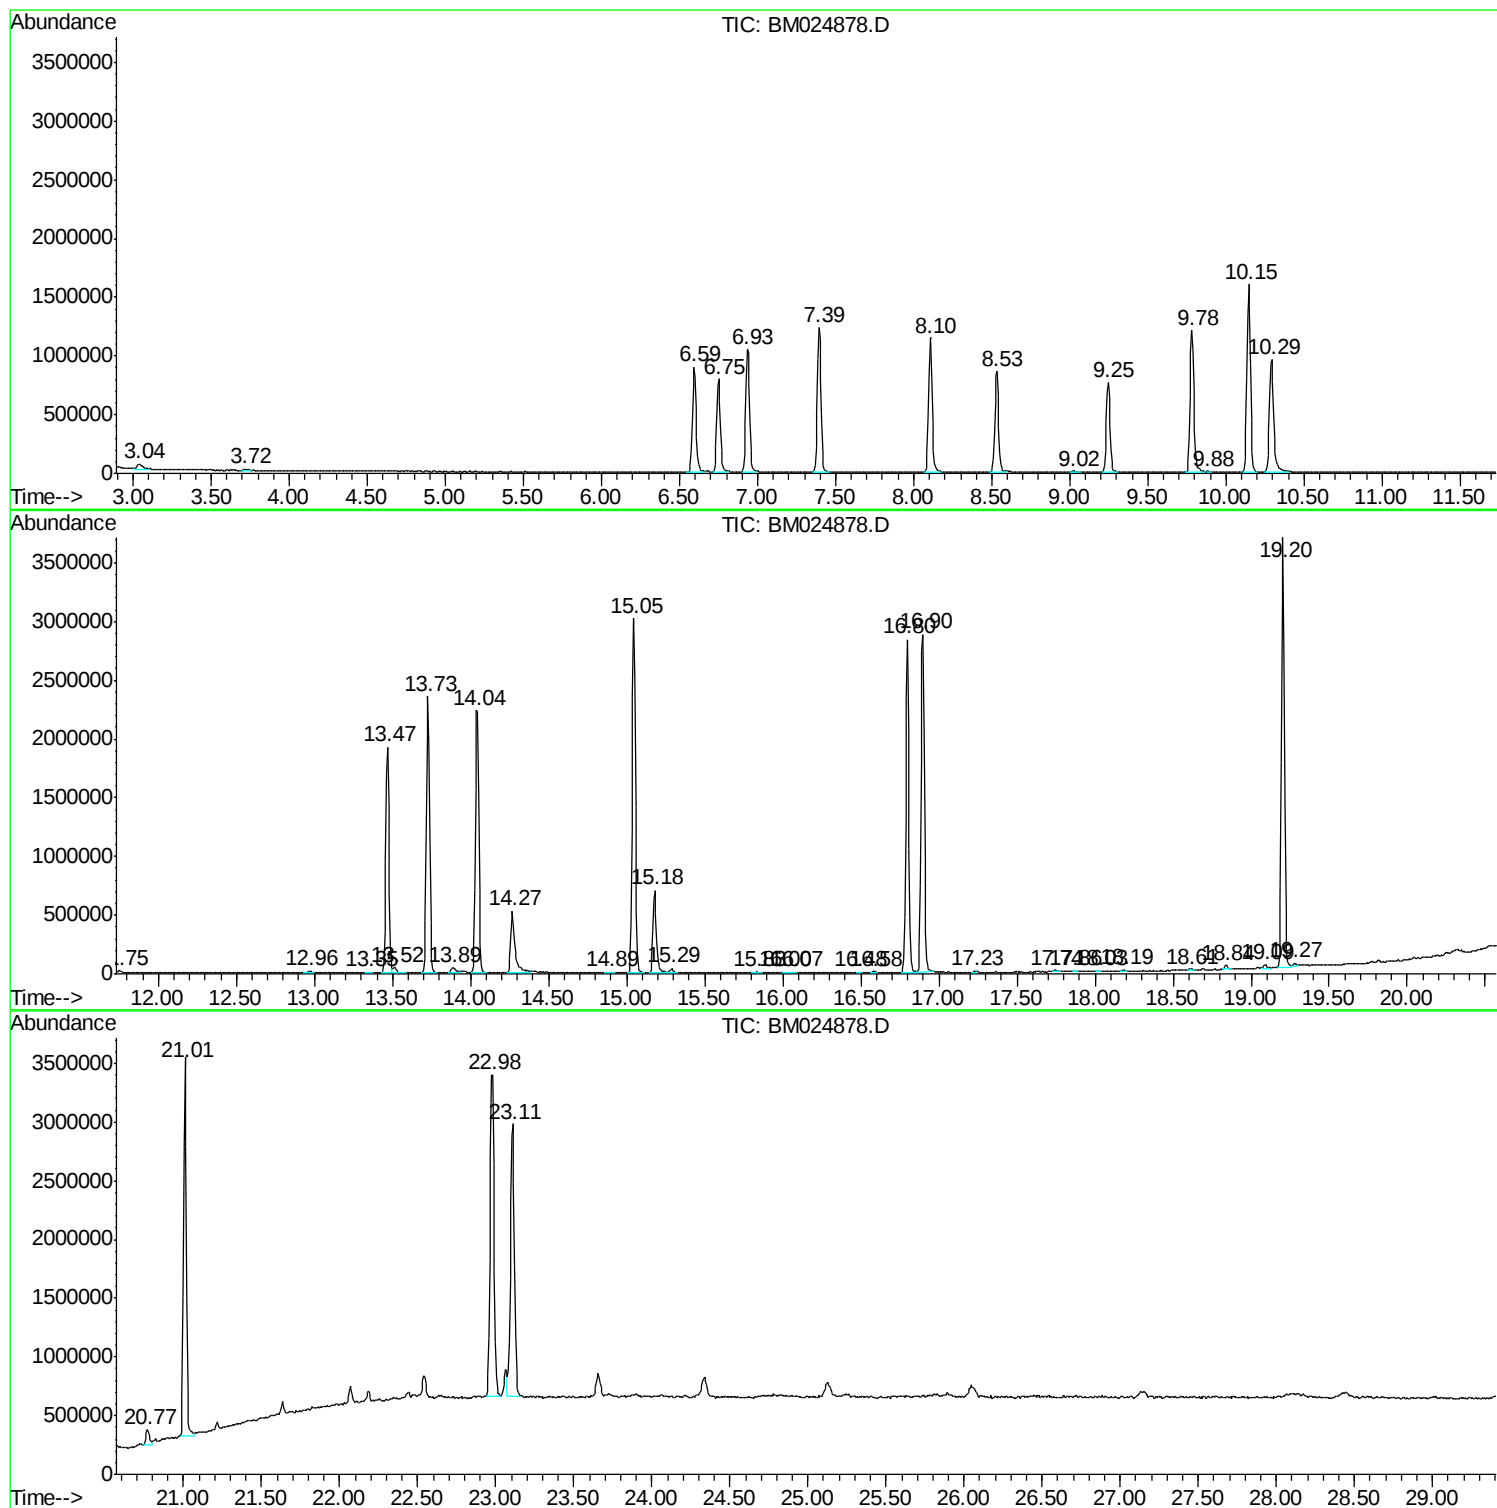

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021320\
Data File : BM024878.D
Acq On : 14 Feb 2020 05:45
Operator : CG/JU
Sample : L1404-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB6Y0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM021320\
Data File : BM024878.D
Acq On : 14 Feb 2020 05:45
Operator : CG/JU
Sample : L1404-20
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB6Y0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM020620MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc