
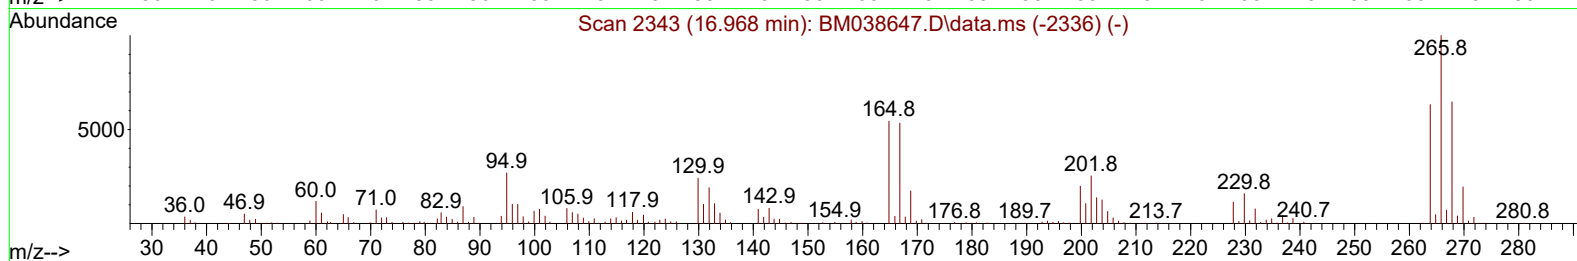
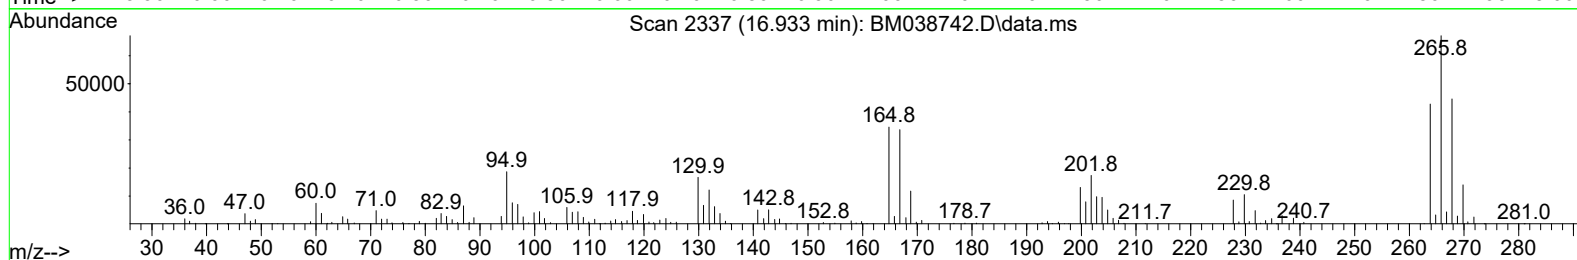


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021523\
Data File : BM038742.D
Acq On : 15 Feb 2023 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 04:16:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 15 02:07:17 2023
Response via : Initial Calibration

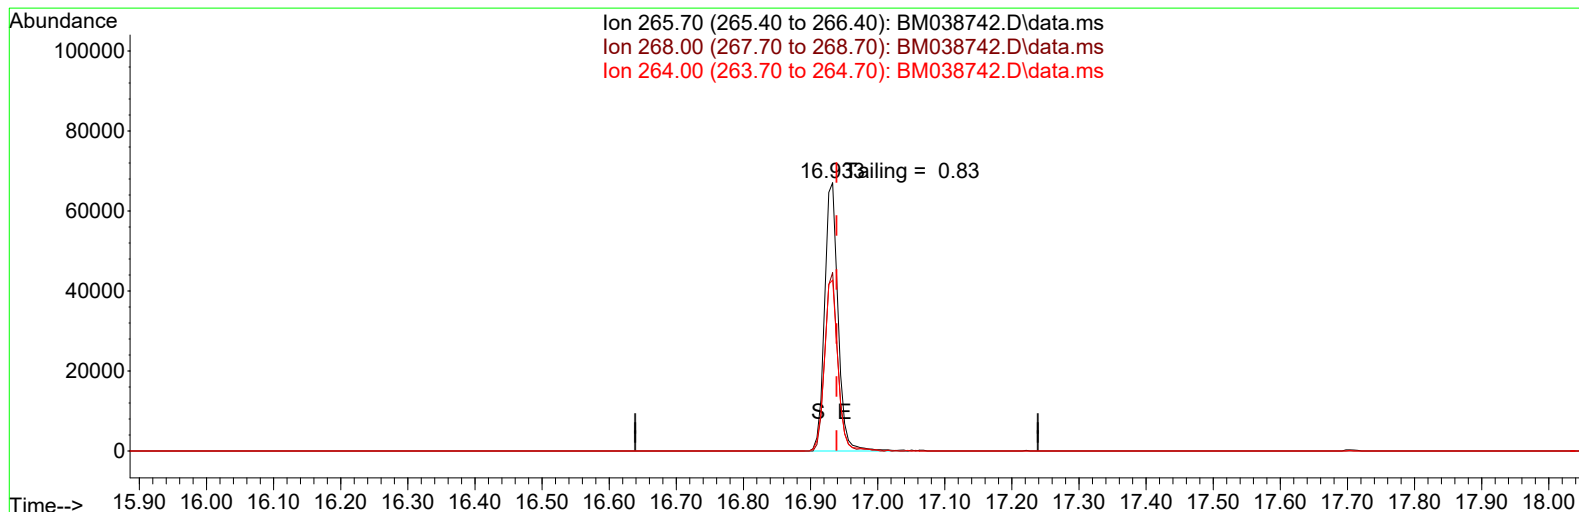

TIC: BM038742.D\data.ms

(70) Pentachlorophenol (C)




16.933min (-0.006) 0.00 ng

response 93780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	66.50
264.00	63.30	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021523\
Data File : BM038742.D
Acq On : 15 Feb 2023 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 04:16:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 15 02:07:17 2023
Response via : Initial Calibration

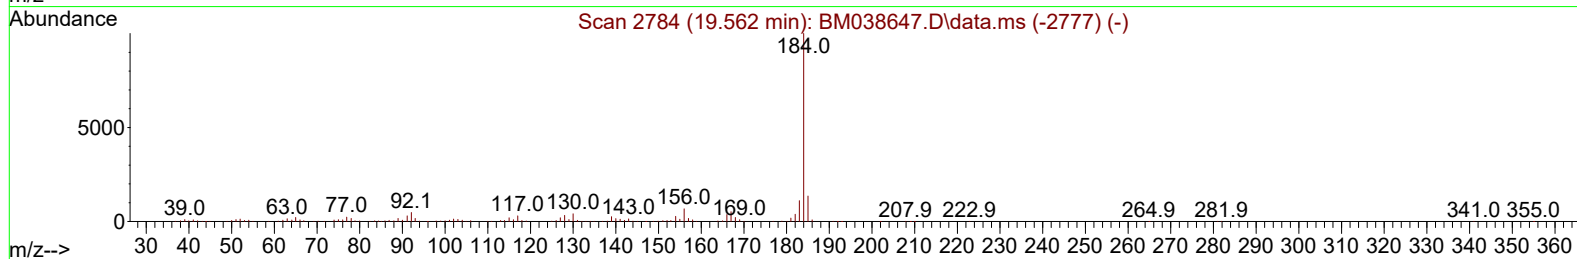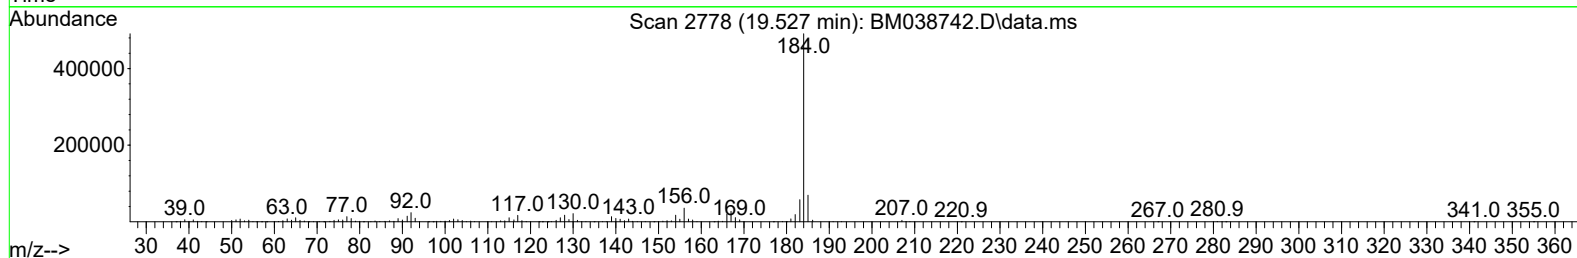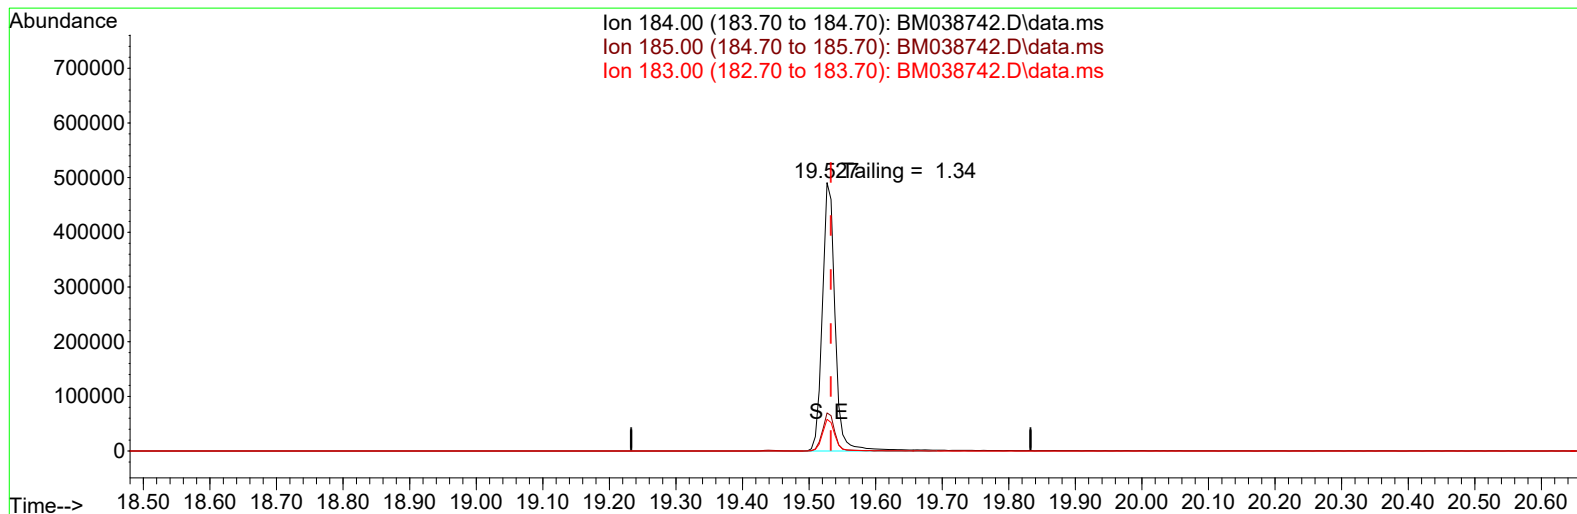

TIC: BM038742.D\data.ms

(77) Benzidine

19.527min (-0.006) 106450.95 ng

response 653209

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.18
183.00	11.00	11.82
0.00	0.00	0.00