
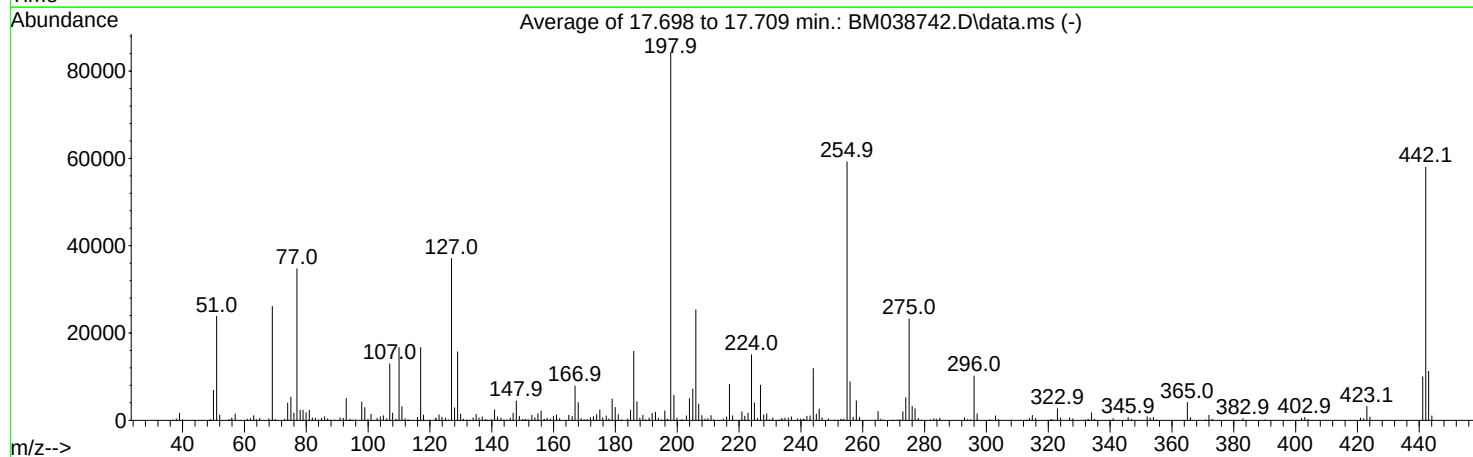


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021523\
Data File : BM038742.D
Acq On : 15 Feb 2023 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 15 02:07:17 2023

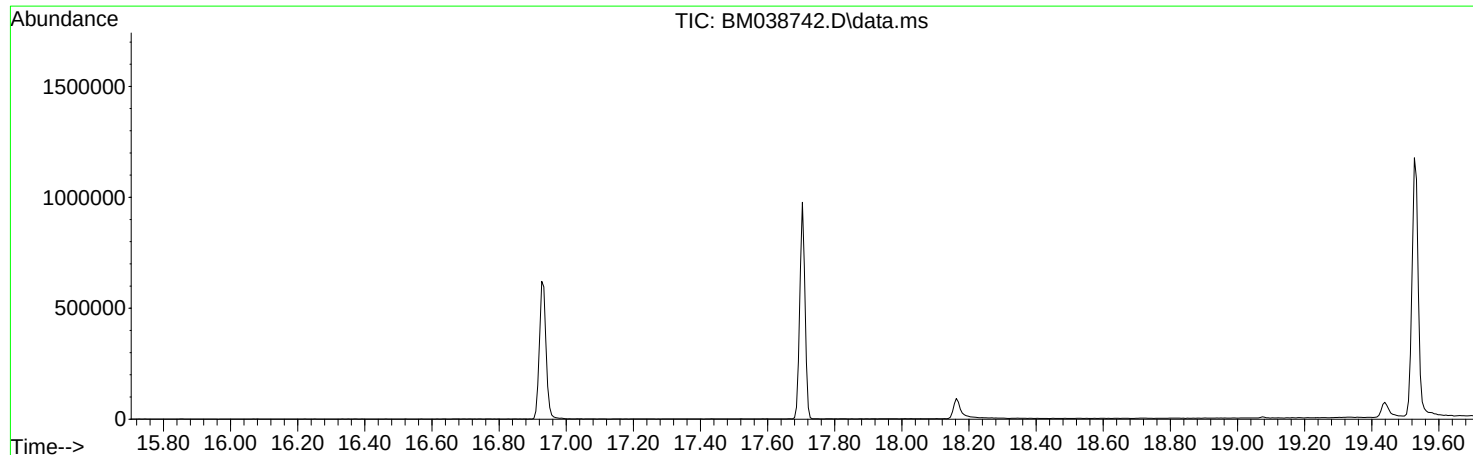




AutoFind: Scans 2467, 2468, 2469; Background Corrected with Scan 2461

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	23824	PASS
68	69	0.00	2	1.3	347	PASS
69	198	0.00	100	30.9	26083	PASS
70	69	0.00	2	0.8	209	PASS
127	198	10	80	44.0	37056	PASS
197	198	0.00	2	0.3	291	PASS
198	198	100	100	100.0	84283	PASS
199	198	5	9	6.8	5752	PASS
275	198	10	60	27.6	23264	PASS
365	198	1	100	4.8	4073	PASS
441	198	0.01	100	11.8	9980	PASS
442	442	50	100	100.0	57965	PASS
443	442	15	24	19.3	11188	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021523\
Data File : BM038742.D
Acq On : 15 Feb 2023 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 16 04:16:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 15 02:07:17 2023
Response via : Initial Calibration

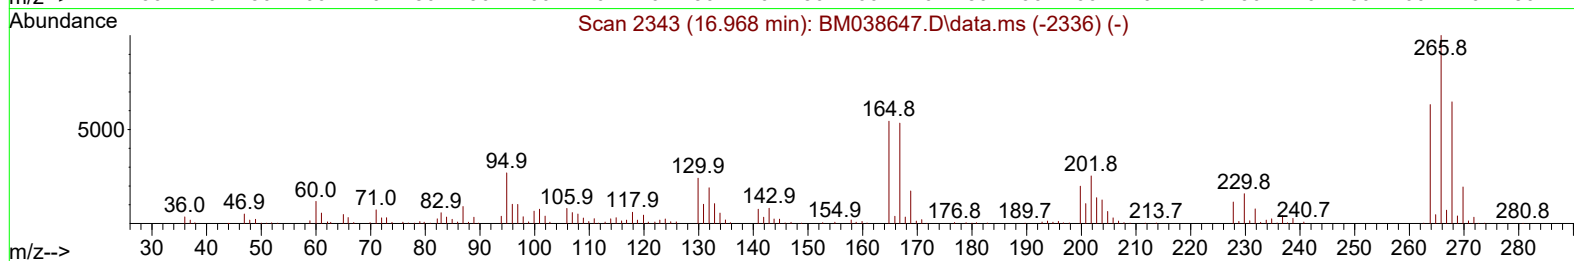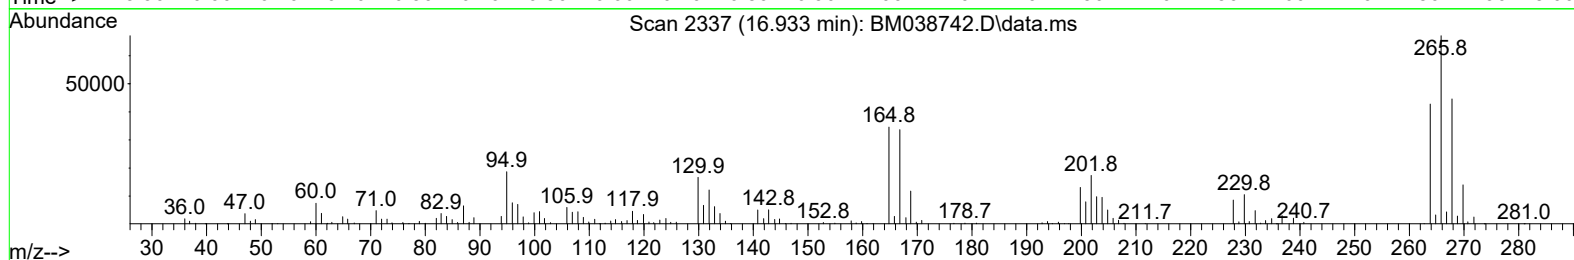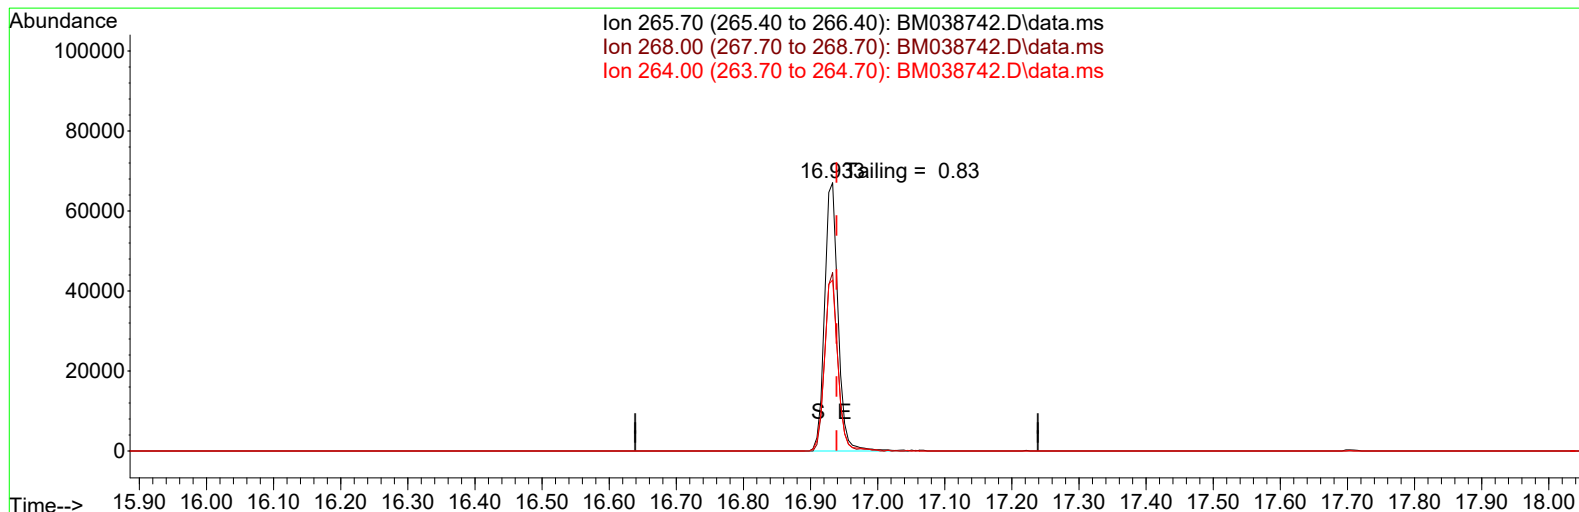

TIC: BM038742.D\data.ms

(70) Pentachlorophenol (C)

16.933min (-0.006) 0.00 ng




response 93780

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	66.50
264.00	63.30	63.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021523\
Data File : BM038742.D
Acq On : 15 Feb 2023 10:56
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 16 04:16:48 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 15 02:07:17 2023
Response via : Initial Calibration

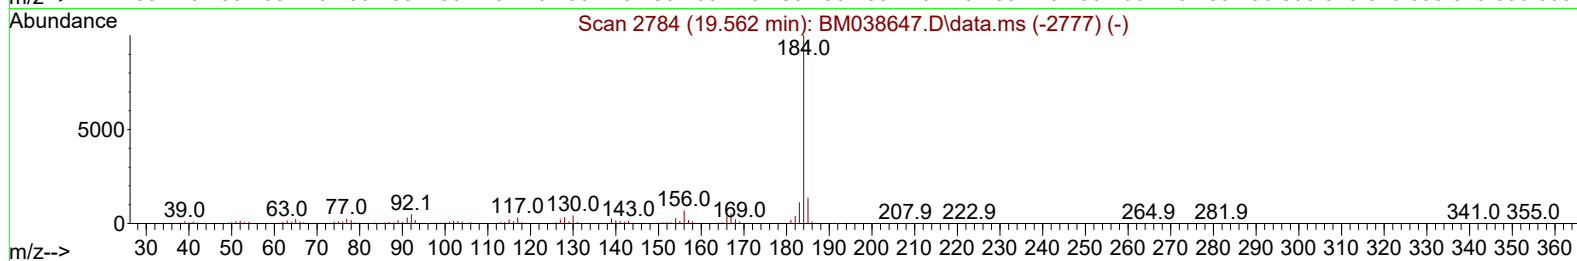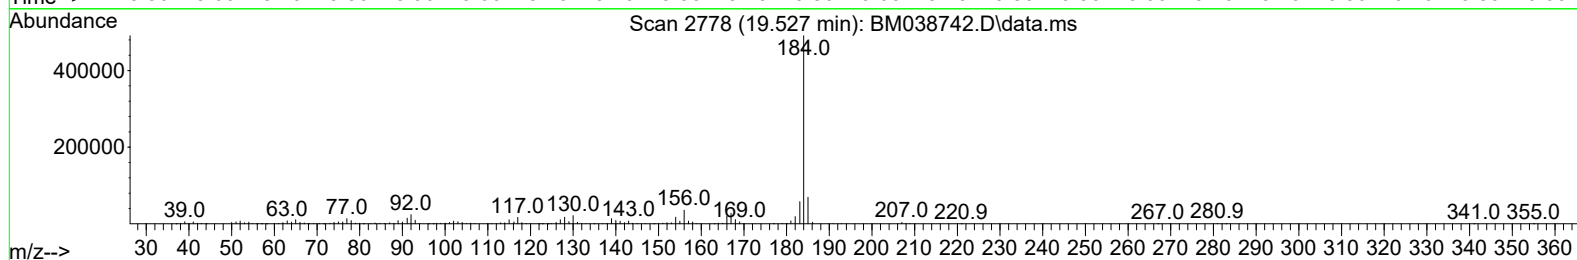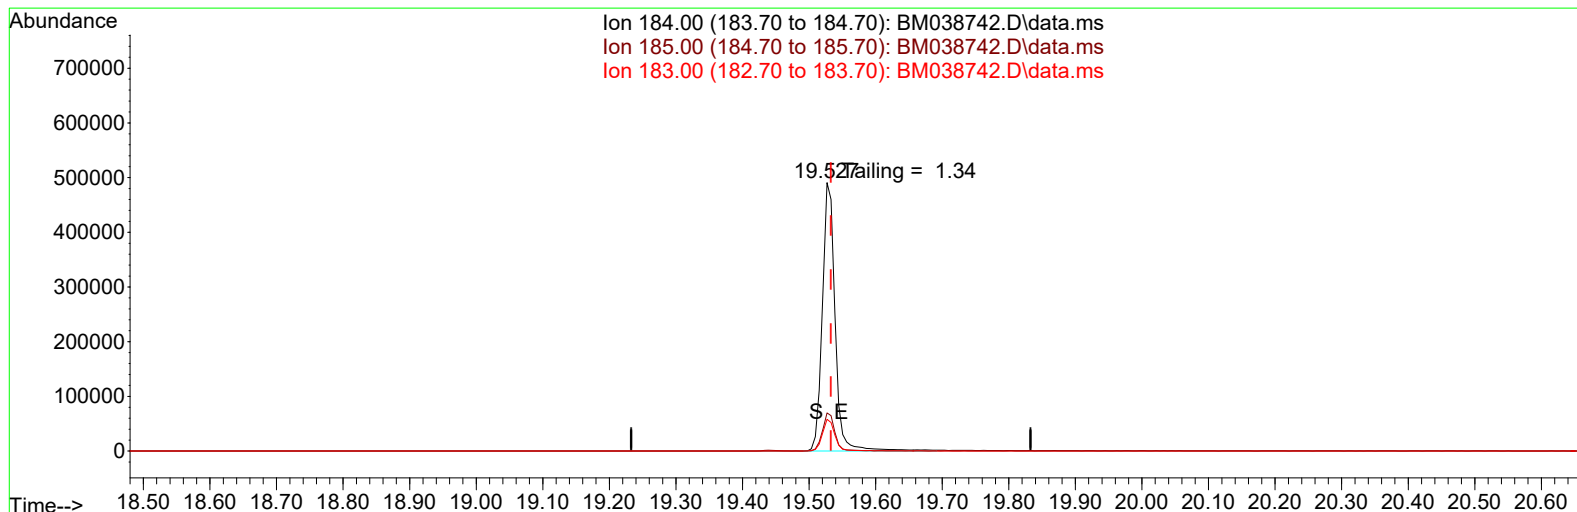

TIC: BM038742.D\data.ms

(77) Benzidine

19.527min (-0.006) 106450.95 ng

response 653209

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.18
183.00	11.00	11.82
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/15/2023	BNA_M	<u>BM038742.D</u>
Compound Name	Response	Retention Time
DDT	309238	20.75
DDD	3190	20.362
DDE	237	19.803
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3427	312665	1.10

Instrument :
BNA_M
ClientSampleId :
DFTPP