


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021723\
Data File : BM038772.D
Acq On : 17 Feb 2023 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 17 23:12:31 2023

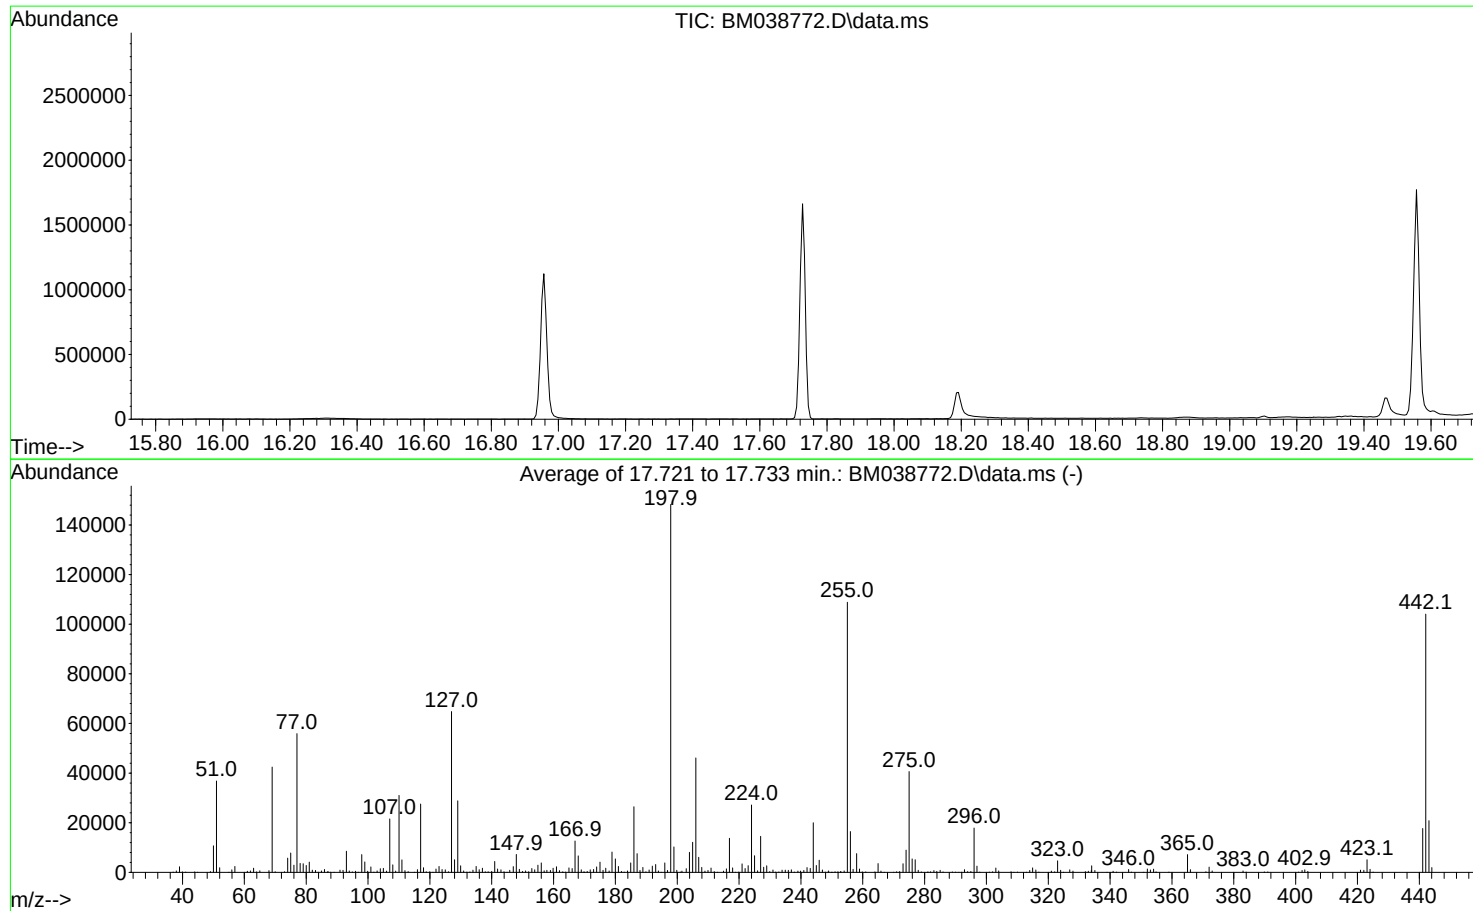




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.8	36821	PASS
68	69	0.00	2	1.7	703	PASS
69	198	0.00	100	28.6	42427	PASS
70	69	0.00	2	0.6	262	PASS
127	198	10	80	43.7	64779	PASS
197	198	0.00	2	0.5	770	PASS
198	198	100	100	100.0	148240	PASS
199	198	5	9	6.9	10279	PASS
275	198	10	60	27.4	40624	PASS
365	198	1	100	4.8	7160	PASS
441	198	0.01	100	11.9	17688	PASS
442	442	50	100	100.0	104091	PASS
443	442	15	24	20.0	20809	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021723\
Data File : BM038772.D
Acq On : 17 Feb 2023 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 18 04:11:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 23:12:31 2023
Response via : Initial Calibration

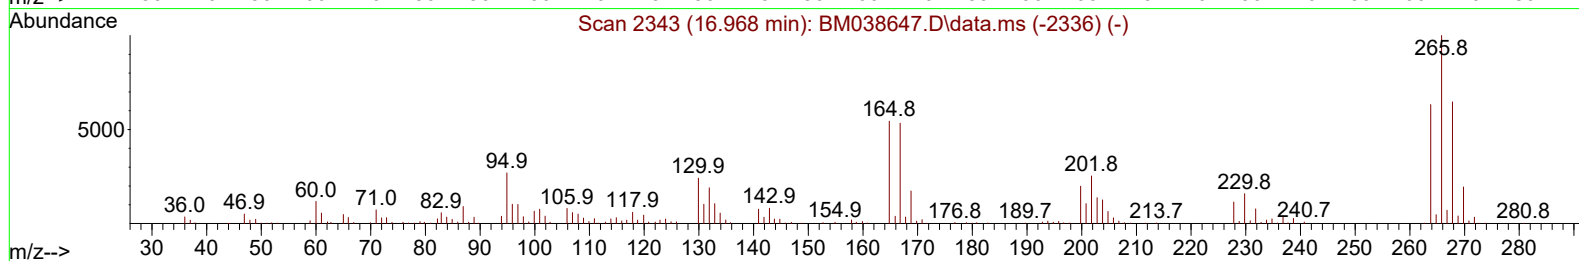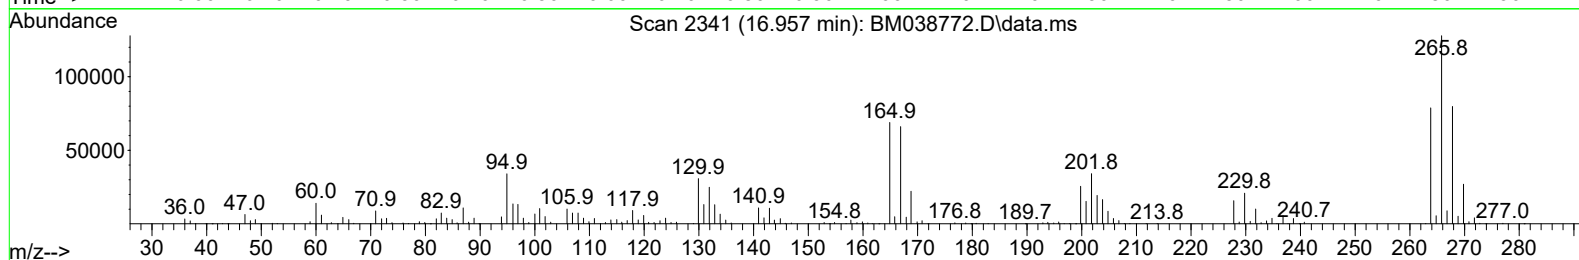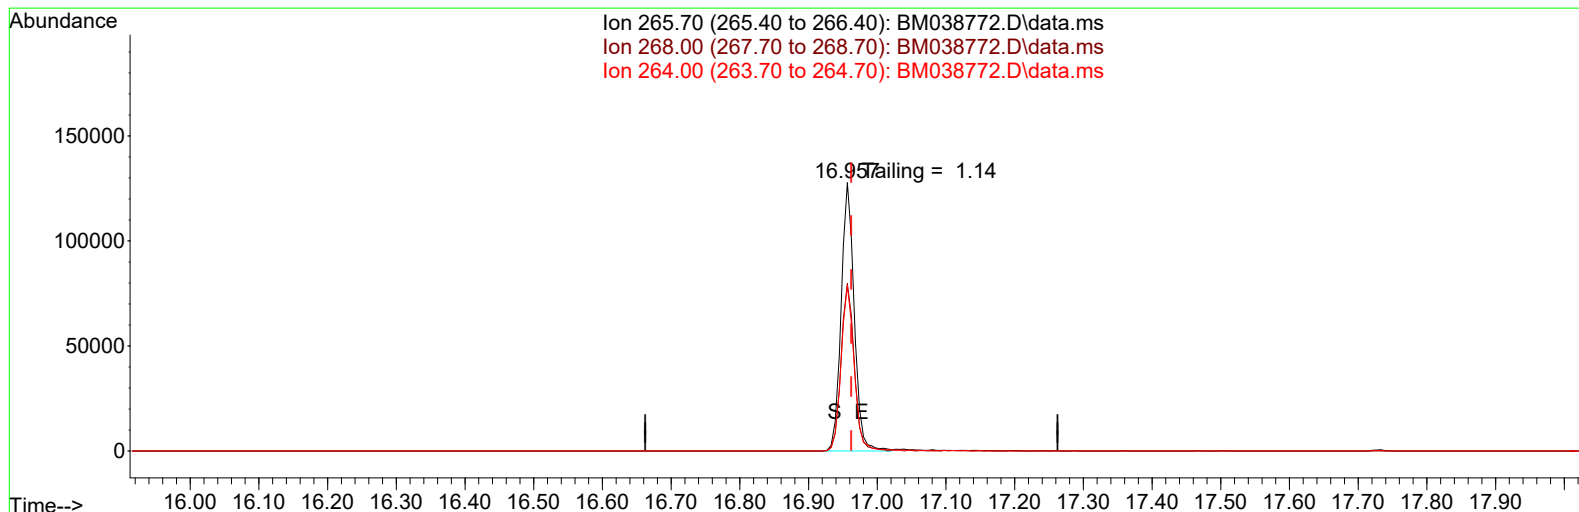

TIC: BM038772.D\data.ms

(70) Pentachlorophenol (C)

16.957min (-0.006) 0.00 ng




response 169068

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	62.41
264.00	63.30	61.63
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM021723\  
Data File : BM038772.D  
Acq On    : 17 Feb 2023   09:44  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 18 04:11:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM020123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Qlast Update : Fri Feb 17 23:12:31 2023
Response via : Initial Calibration

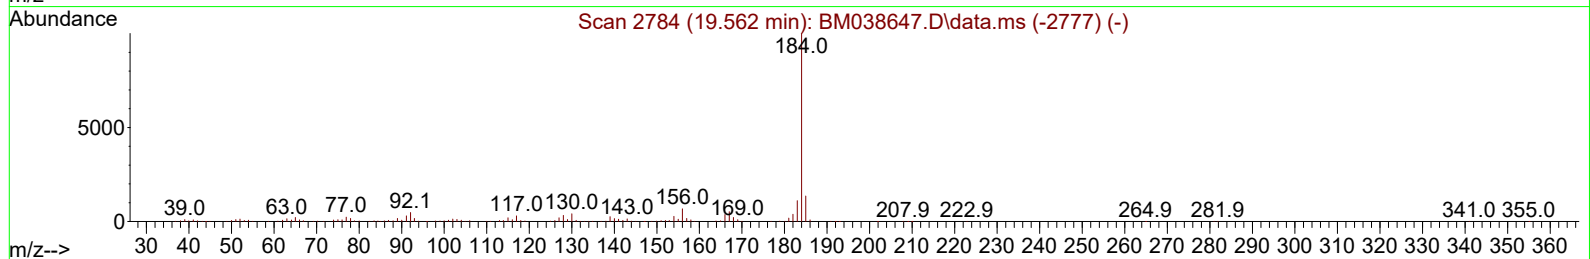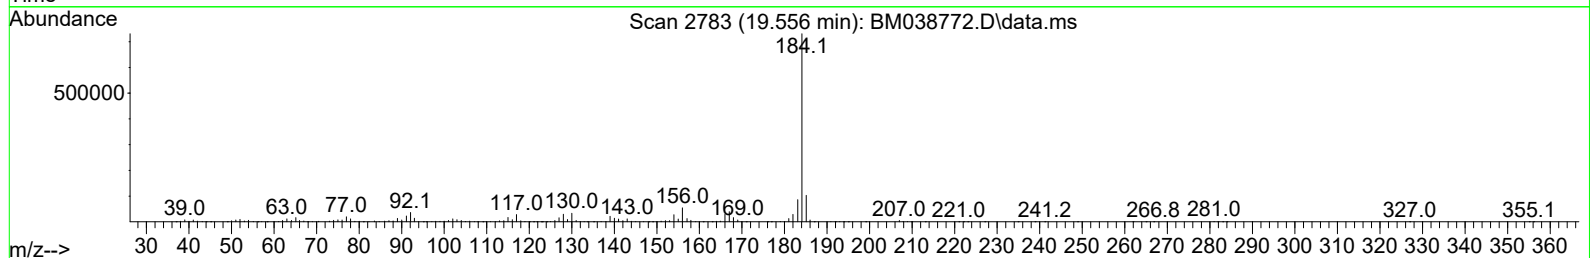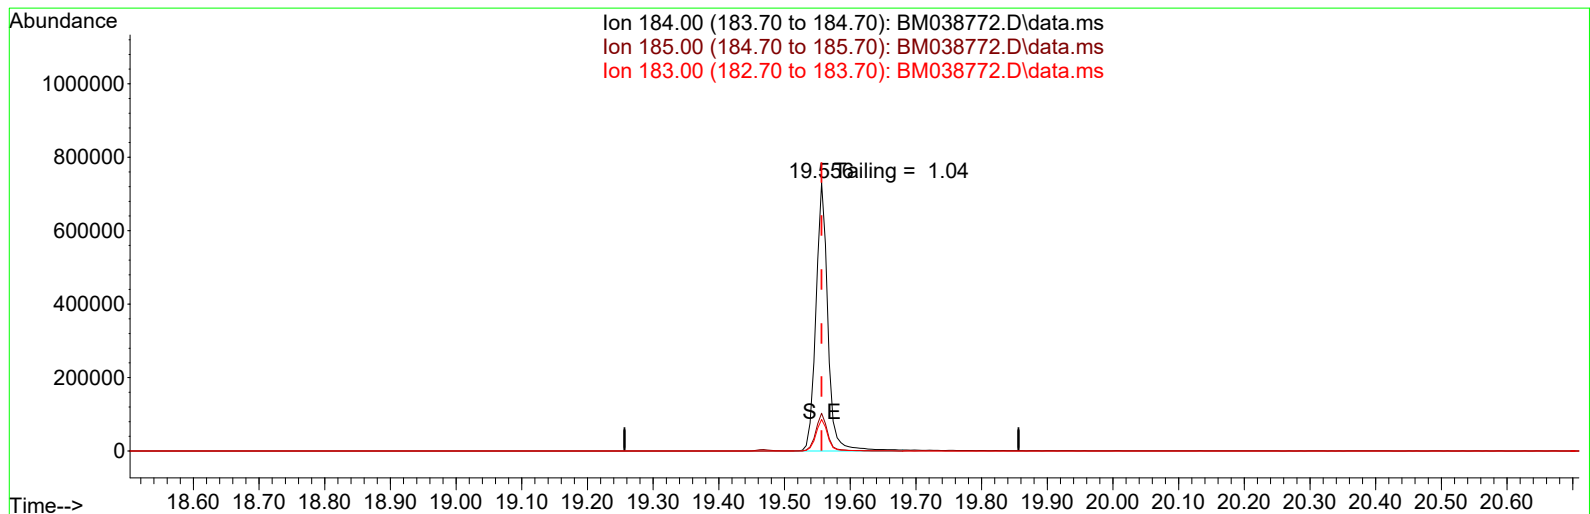

TIC: BM038772.D\data.ms

(77) Benzidine

19.556min (-0.000) 27421.14 ng

response **932855**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.07
183.00	11.00	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/17/2023	BNA_M	<u>BM038772.D</u>
Compound Name	Response	Retention Time
DDT	535261	20.774
DDD	6411	20.386
DDE	134	19.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6545	541806	1.21

Instrument :
BNA_M
ClientSampleId :
DFTPP