
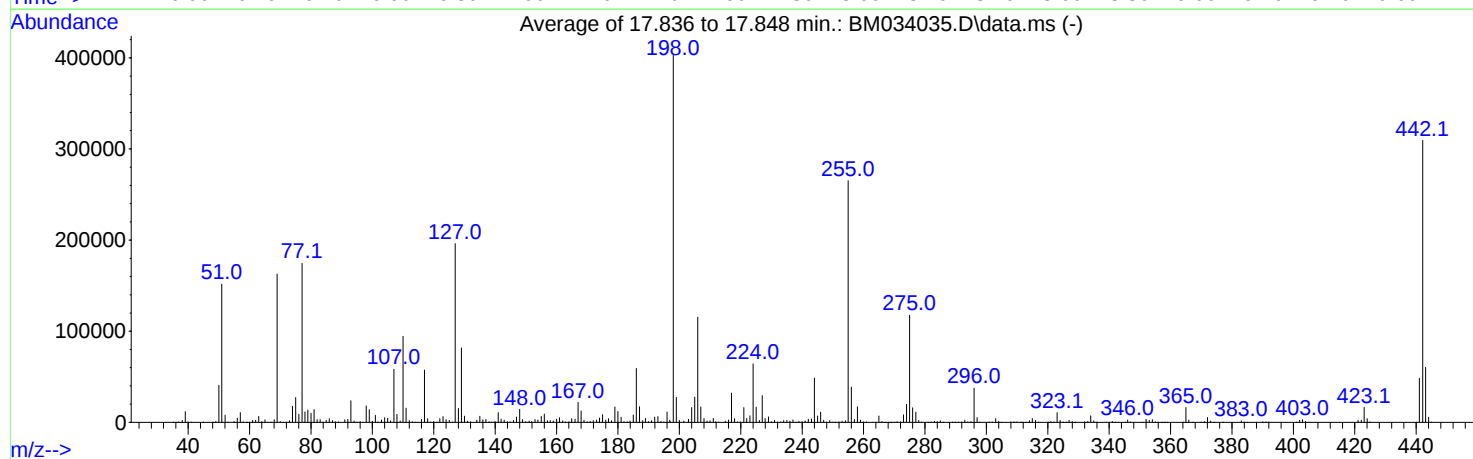


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022222\
 Data File : BM034035.D
 Acq On : 22 Feb 2022 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 22 17:55:56 2022

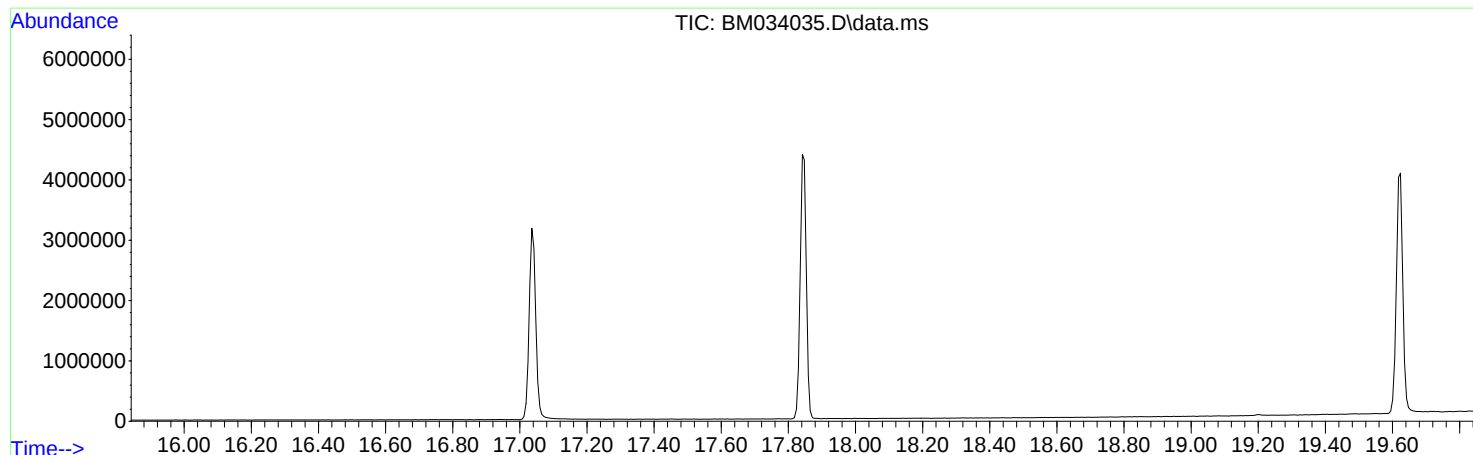




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.6	151760	PASS
68	69	0.00	2	1.8	2965	PASS
69	198	0.00	100	40.3	162709	PASS
70	69	0.00	2	0.5	891	PASS
127	198	10	80	48.6	196139	PASS
197	198	0.00	2	0.6	2246	PASS
198	198	100	100	100.0	403669	PASS
199	198	5	9	6.8	27477	PASS
275	198	10	60	29.1	117480	PASS
365	198	1	100	4.0	16271	PASS
441	198	0.01	100	11.9	48213	PASS
442	442	50	100	100.0	309333	PASS
443	442	15	24	19.5	60435	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022222\
 Data File : BM034035.D
 Acq On : 22 Feb 2022 11:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Feb 22 13:47:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 22 13:47:12 2022
 Response via : Initial Calibration

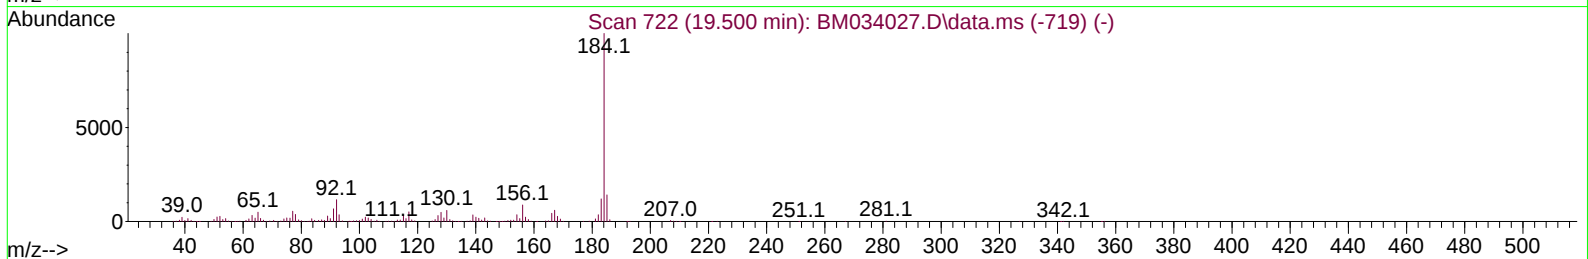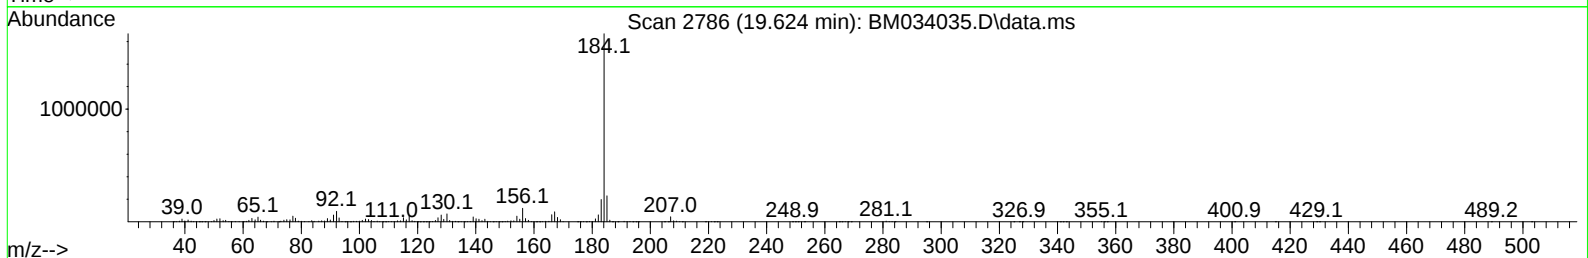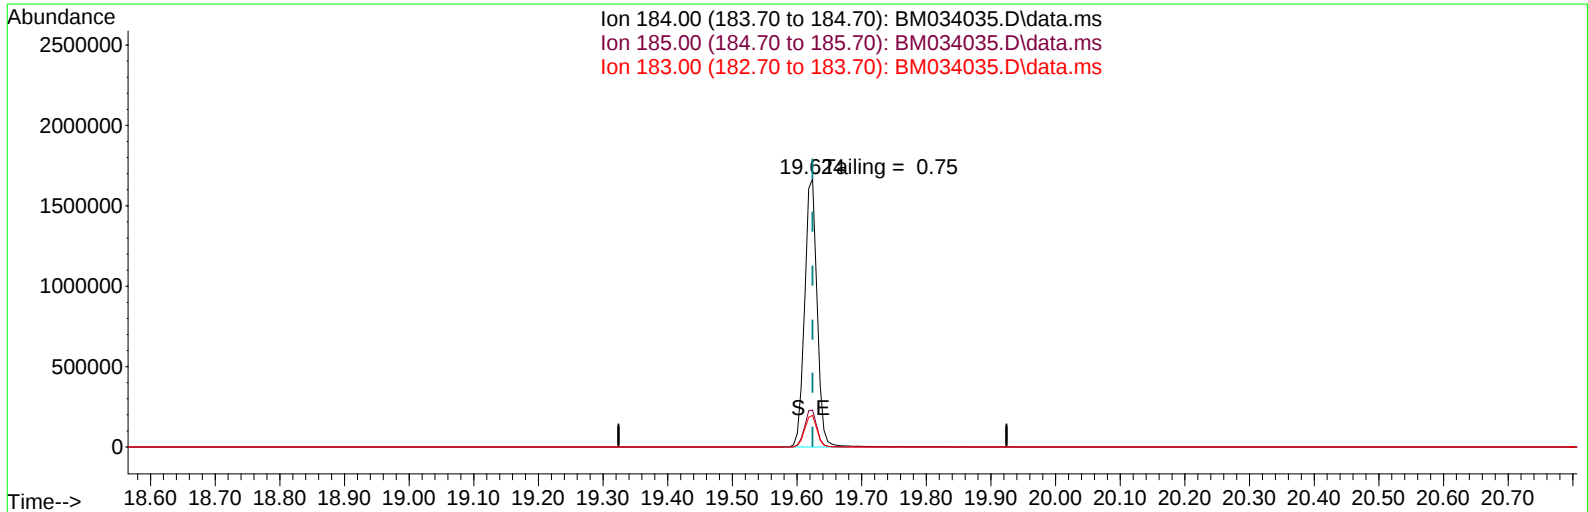

TIC: BM034035.D\data.ms

(77) Benzidine**19.624min (0.000) 6419.54 ng****response 2238960**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.78
183.00	12.10	11.85
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/22/2022	BNA_M	<u>BM034035.D</u>
Compound Name	Response	Retention Time
DDT	1320402	20.86
DDD	5605	20.41
DDE	1139	19.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6744	1327146	0.51

Instrument :
BNA_M
ClientSampleId :
DFTPP