

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022422\
 Data File : BM034065.D
 Acq On : 24 Feb 2022 12:15
 Operator : CG/JU
 Sample : PB142854BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB142854BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034065.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.566	389	396	406	rBV	4073872	5732000	52.52%	10.969%
2	7.166	659	668	678	rBV	3770389	5732513	52.52%	10.970%
3	8.013	805	812	820	rBV	791088	1227577	11.25%	2.349%
4	9.178	1002	1010	1020	rBV	2285290	3726199	34.14%	7.131%
5	10.831	1283	1291	1299	rVB	940613	1560286	14.30%	2.986%
6	13.277	1700	1707	1718	rBV	6081707	8923183	81.76%	17.076%
7	14.648	1933	1940	1953	rBV	1378144	1978914	18.13%	3.787%
8	16.130	2185	2192	2213	rBV	4311699	6133751	56.20%	11.738%
9	17.389	2399	2406	2412	rBV	1521815	2160511	19.80%	4.135%
10	20.006	2845	2851	2859	rBV	9030634	10914230	100.00%	20.886%
11	21.559	3110	3115	3120	rBV	1665645	2064559	18.92%	3.951%
12	24.018	3527	3533	3545	rVB2	1004866	2101918	19.26%	4.022%




Sum of corrected areas: 52255641

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022422\
Data File : BM034065.D
Acq On : 24 Feb 2022 12:15
Operator : CG/JU
Sample : PB142854BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142854BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

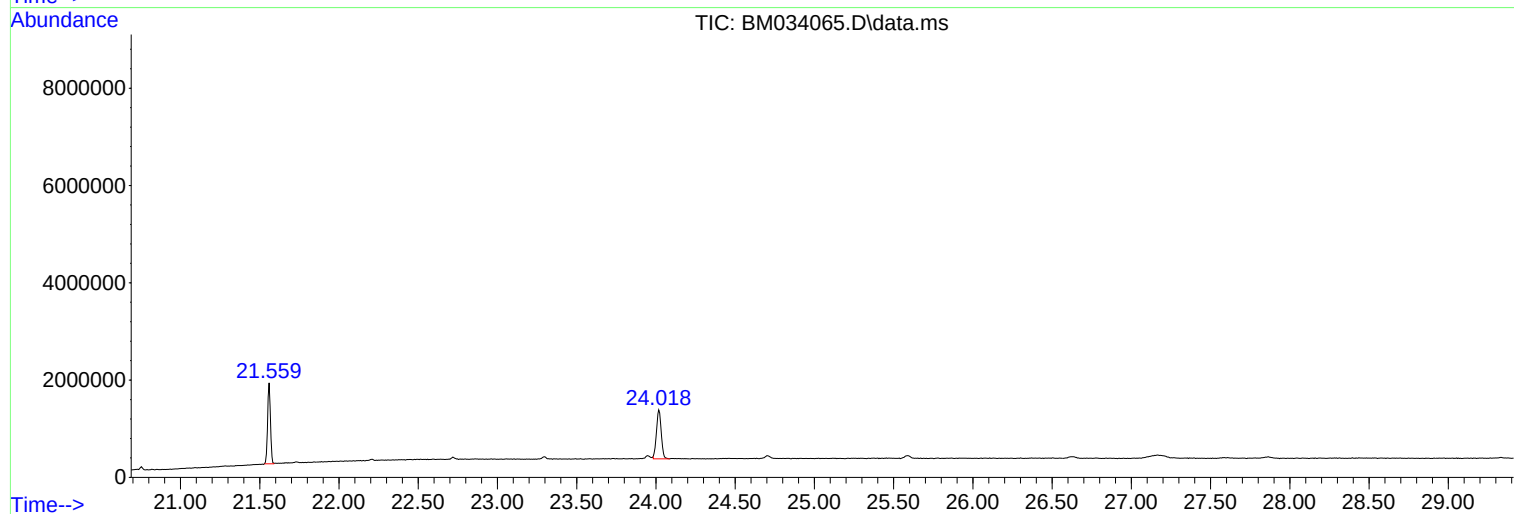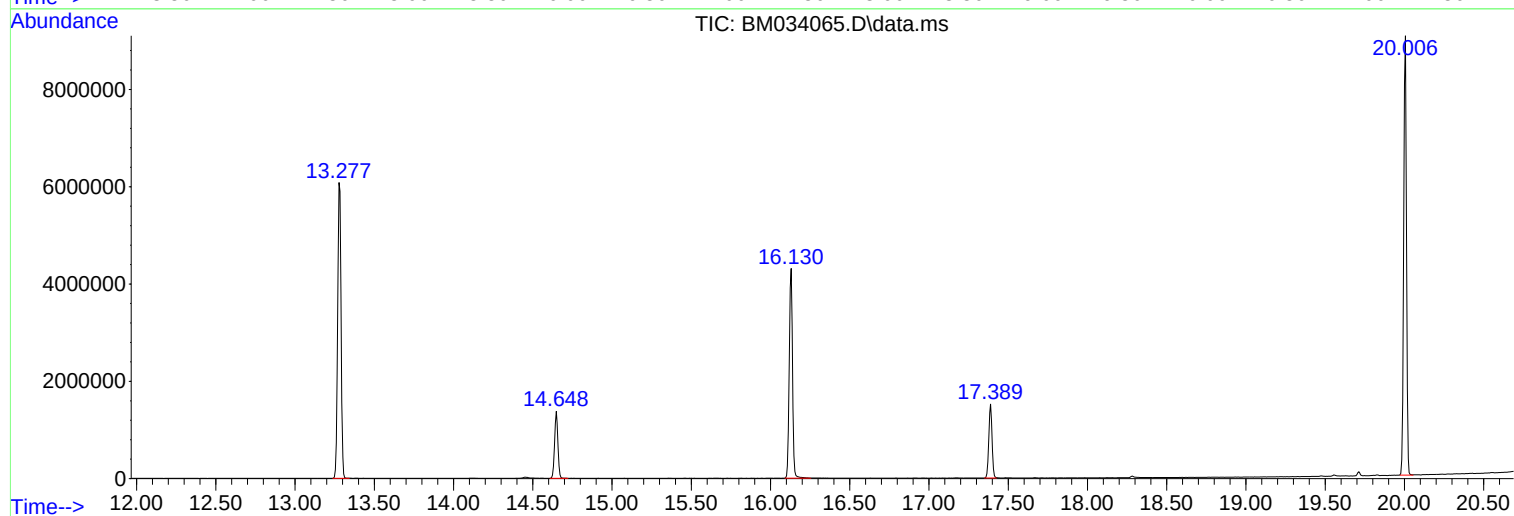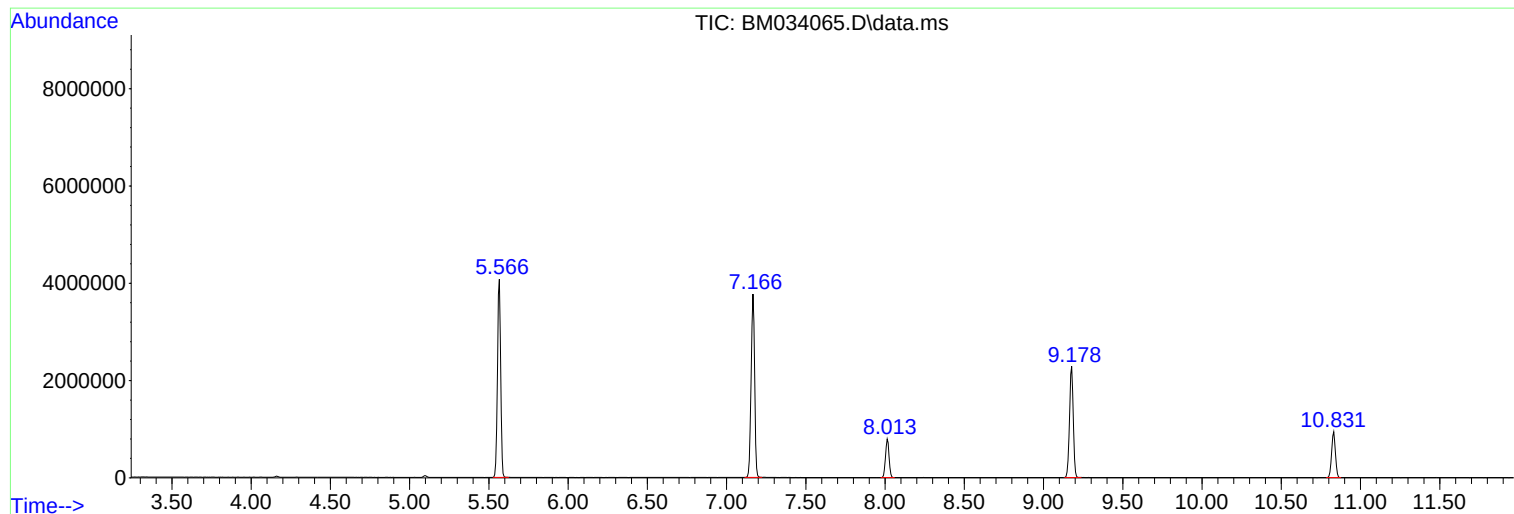

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022422\
Data File : BM034065.D
Acq On : 24 Feb 2022 12:15
Operator : CG/JU
Sample : PB142854BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142854BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022422\
Data File : BM034065.D
Acq On : 24 Feb 2022 12:15
Operator : CG/JU
Sample : PB142854BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB142854BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------