

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM022422\  
 Data File : BM034067.D  
 Acq On : 24 Feb 2022 14:58  
 Operator : CG/JU  
 Sample : PB142897BL  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB142897BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022222.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034067.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.560       | 388           | 395         | 405          | rBV      | 4190430        | 5955953       | 43.53%          | 10.134%       |
| 2         | 7.166       | 659           | 668         | 680          | rBV      | 3899523        | 6065593       | 44.33%          | 10.321%       |
| 3         | 8.013       | 804           | 812         | 821          | rVB      | 777169         | 1212387       | 8.86%           | 2.063%        |
| 4         | 9.172       | 1001          | 1009        | 1021         | rBV      | 2336262        | 3852693       | 28.16%          | 6.556%        |
| 5         | 10.830      | 1283          | 1291        | 1298         | rVB      | 945783         | 1584876       | 11.58%          | 2.697%        |
| 6         | 13.277      | 1700          | 1707        | 1723         | rBV      | 6583694        | 9746583       | 71.23%          | 16.584%       |
| 7         | 14.648      | 1934          | 1940        | 1950         | rBV      | 1504185        | 2140169       | 15.64%          | 3.642%        |
| 8         | 16.130      | 2185          | 2192        | 2209         | rBV      | 5177243        | 7182683       | 52.49%          | 12.222%       |
| 9         | 17.389      | 2399          | 2406        | 2417         | rBV      | 1788285        | 2526582       | 18.47%          | 4.299%        |
| 10        | 20.006      | 2845          | 2851        | 2861         | rBV      | 11413879       | 13682762      | 100.00%         | 23.282%       |
| 11        | 21.559      | 3110          | 3115        | 3121         | rBV      | 1984687        | 2470390       | 18.05%          | 4.204%        |
| 12        | 24.018      | 3527          | 3533        | 3546         | rVB2     | 1135131        | 2348808       | 17.17%          | 3.997%        |


Sum of corrected areas: 58769479

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM022422\  
Data File : BM034067.D  
Acq On : 24 Feb 2022 14:58  
Operator : CG/JU  
Sample : PB142897BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB142897BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

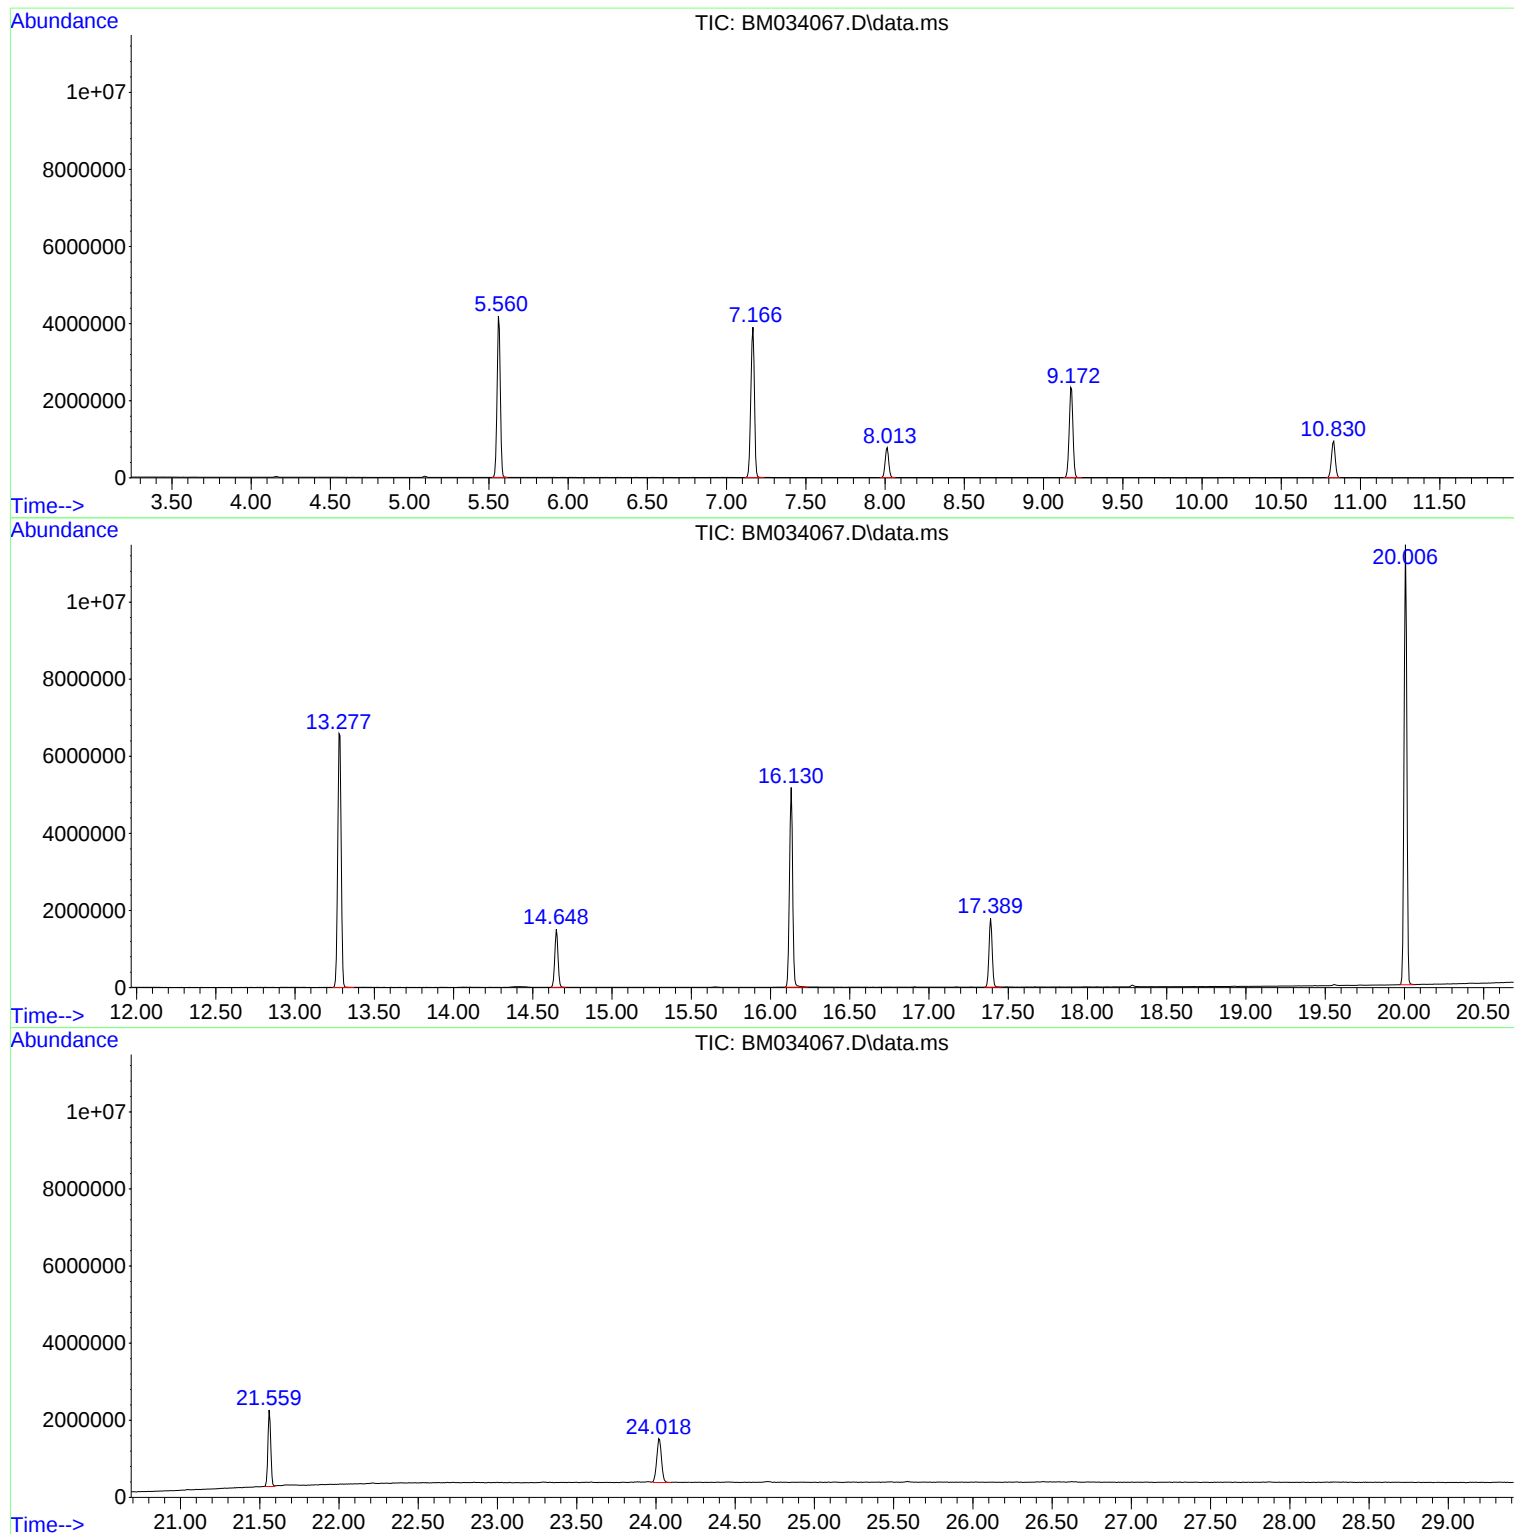

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM022422\  
Data File : BM034067.D  
Acq On : 24 Feb 2022 14:58  
Operator : CG/JU  
Sample : PB142897BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB142897BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM022422\  
Data File : BM034067.D  
Acq On : 24 Feb 2022 14:58  
Operator : CG/JU  
Sample : PB142897BL  
Misc :  
ALS Vial : 5 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB142897BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM022222.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|