


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022422\
 Data File : BM034063.D
 Acq On : 24 Feb 2022 10:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 22 17:55:56 2022

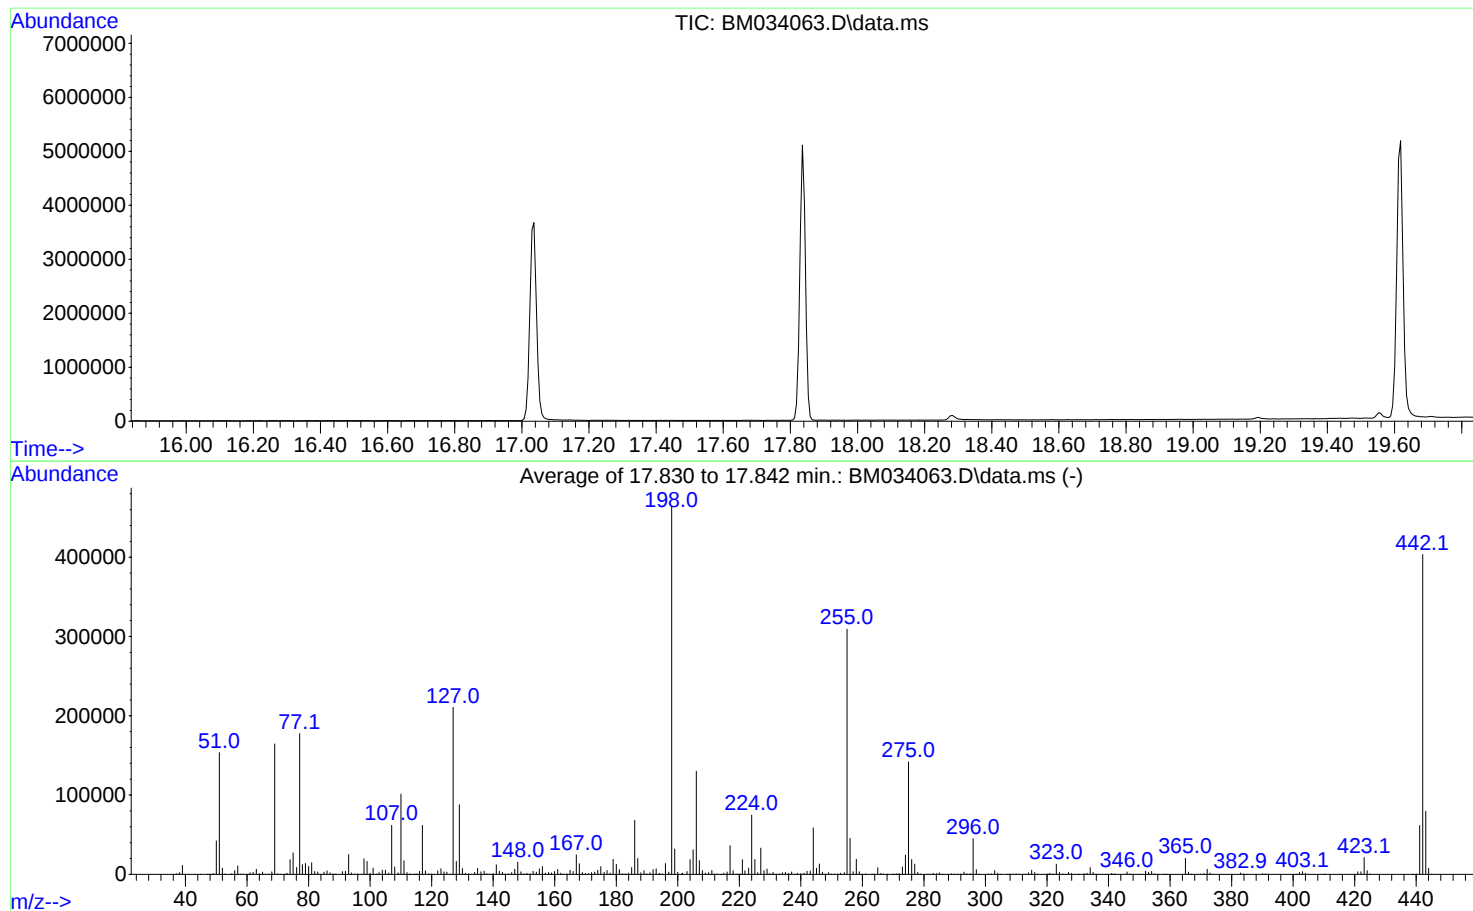




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.1	153560	PASS
68	69	0.00	2	1.9	3177	PASS
69	198	0.00	100	35.4	164395	PASS
70	69	0.00	2	0.5	836	PASS
127	198	10	80	45.4	210624	PASS
197	198	0.00	2	0.6	2761	PASS
198	198	100	100	100.0	463957	PASS
199	198	5	9	6.9	31947	PASS
275	198	10	60	30.6	141931	PASS
365	198	1	100	4.4	20211	PASS
441	198	0.01	100	13.3	61533	PASS
442	442	50	100	100.0	403499	PASS
443	442	15	24	19.7	79472	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022422\
Data File : BM034063.D
Acq On : 24 Feb 2022 10:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 25 04:28:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 22 17:55:56 2022
Response via : Initial Calibration

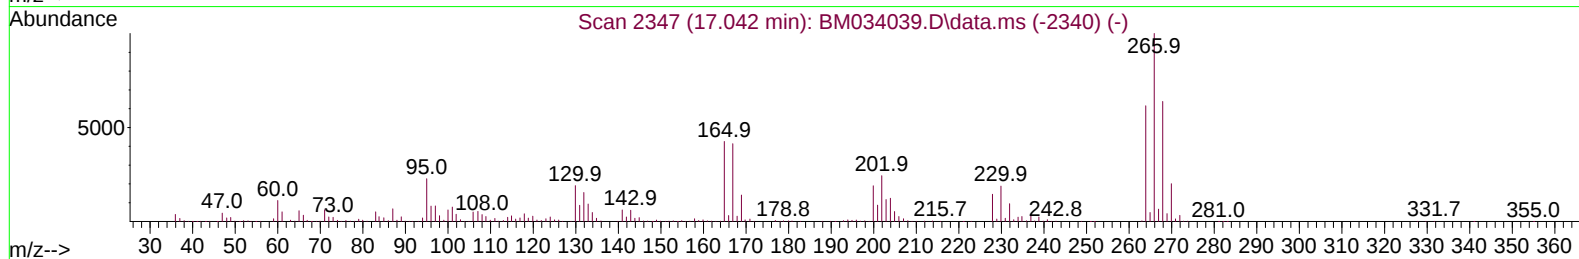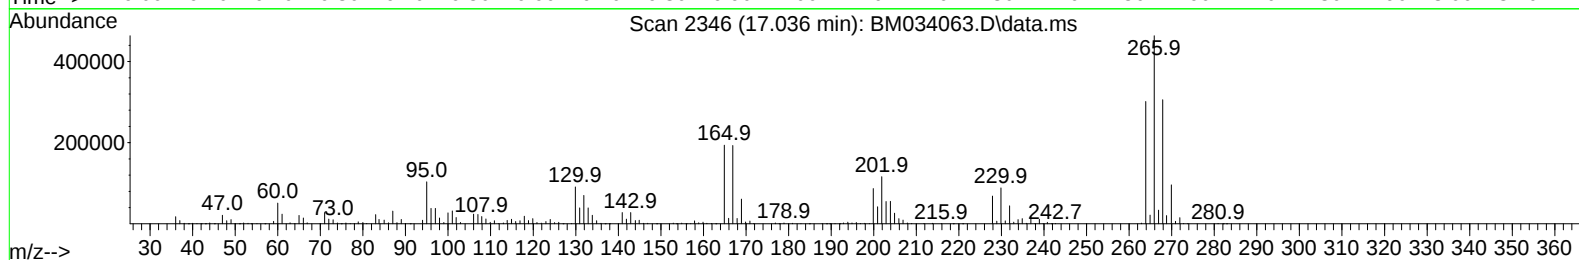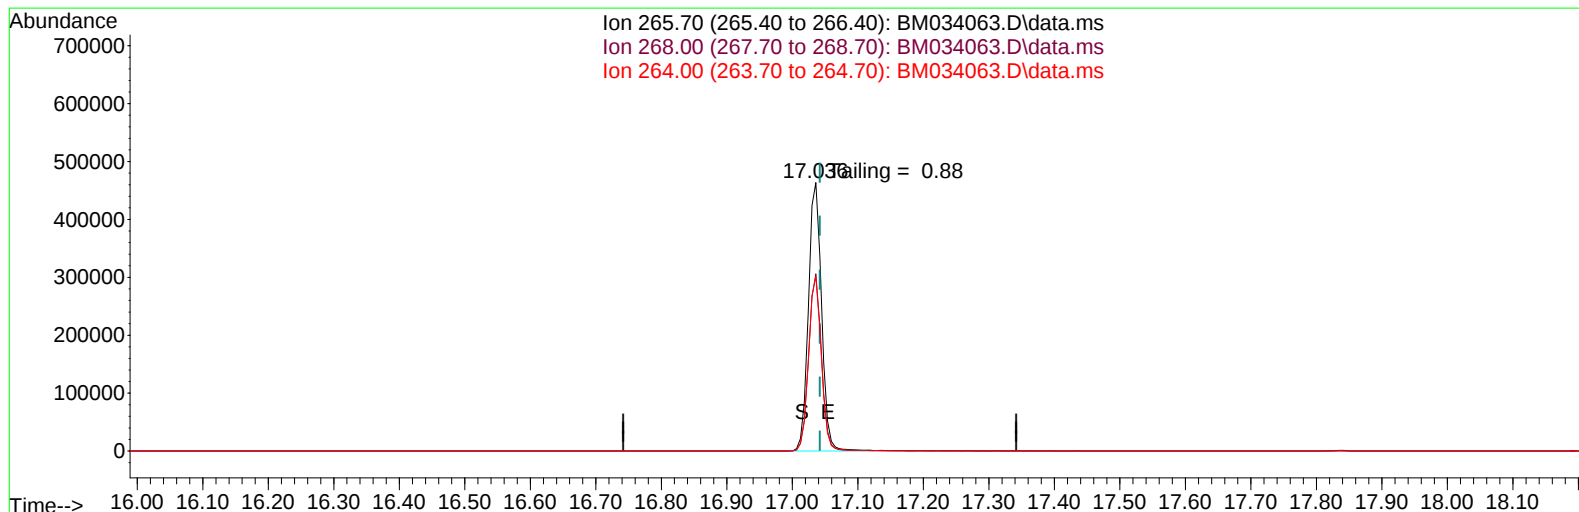

TIC: BM034063.D\data.ms

(70) Pentachlorophenol (C)

17.036min (-0.006) 1494313.95 ng




response 646265

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	66.01
264.00	61.40	65.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM022422\
Data File : BM034063.D
Acq On : 24 Feb 2022 10:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Feb 25 04:28:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 22 17:55:56 2022
Response via : Initial Calibration

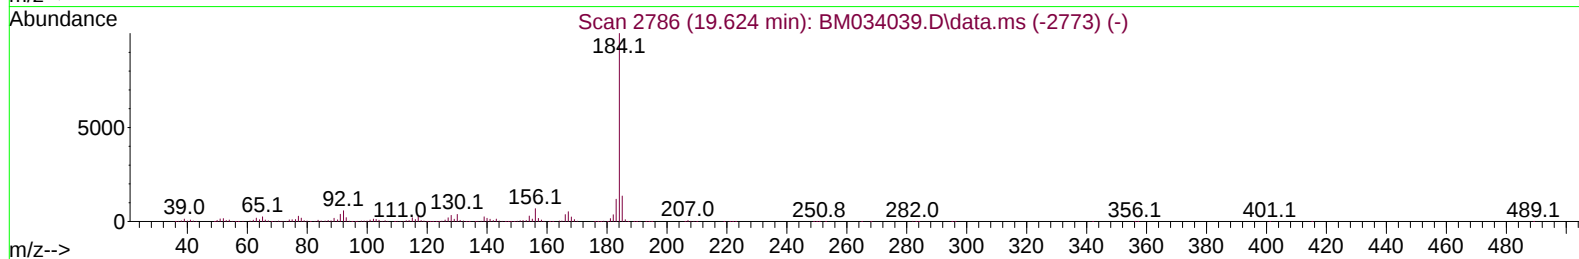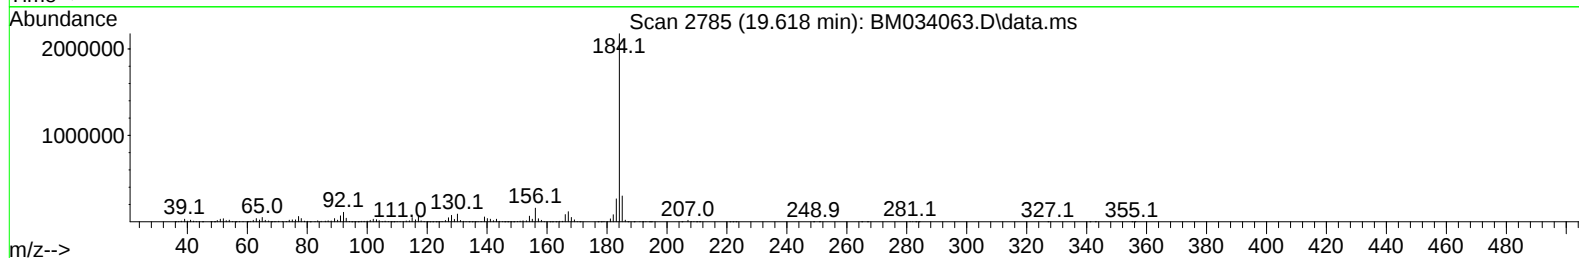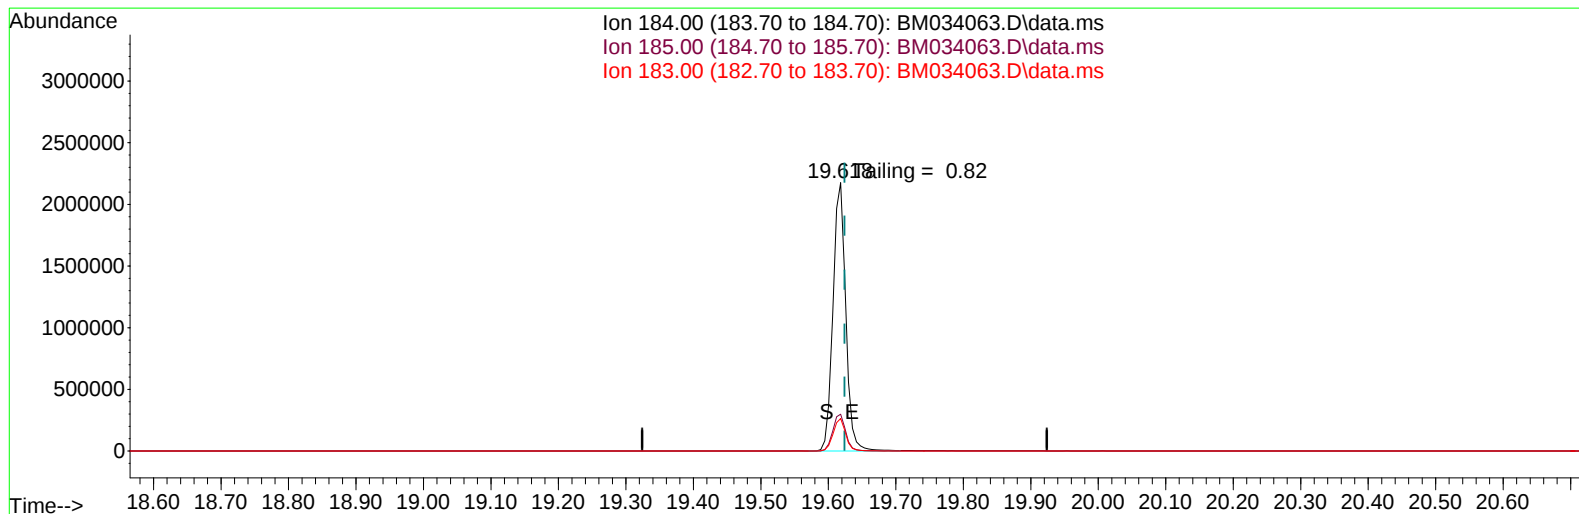

TIC: BM034063.D\data.ms

(77) Benzidine

19.618min (-0.006) 767383.44 ng

response 2858220

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.75
183.00	12.10	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/24/2022	BNA_M	<u>BM034063.D</u>
Compound Name	Response	Retention Time
DDT	1594101	20.853
DDD	18370	20.412
DDE	744	19.912
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19114	1613215	1.18

Instrument :
BNA_M
ClientSampleId :
DFTPP