

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022621\
 Data File : BM028899.D
 Acq On : 25 Feb 2021 16:36
 Operator : CG/JU
 Sample : PB134807BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.146	24	27	33	rVB	4333	5708	1.74%	0.138%
2	3.910	153	157	160	rBB	592	710	0.22%	0.017%
3	6.987	674	680	690	rBB	80017	124853	38.03%	3.027%
4	7.140	700	706	714	rBB	60287	91840	27.97%	2.226%
5	7.334	733	739	746	rBV	88752	134065	40.83%	3.250%
6	7.798	813	818	826	rBB	74933	117540	35.80%	2.849%
7	8.534	937	943	953	rBB	98873	151223	46.06%	3.666%
8	8.975	1012	1018	1027	rBB	75499	121047	36.87%	2.934%
9	9.698	1135	1141	1148	rBB	68027	104978	31.97%	2.545%
10	10.239	1227	1233	1242	rBV	94382	153462	46.74%	3.720%
11	10.604	1288	1295	1304	rBB	105377	164940	50.23%	3.998%
12	10.757	1315	1321	1334	rBB	95995	158161	48.17%	3.834%
13	12.198	1563	1566	1569	rBB	806	1029	0.31%	0.025%
14	13.880	1846	1852	1857	rBV	160926	220250	67.08%	5.339%
15	14.157	1893	1899	1905	rBV	199192	274747	83.68%	6.660%
16	14.463	1945	1951	1957	rBB	148522	207517	63.20%	5.030%
17	14.698	1987	1991	2008	rBB	59297	90970	27.71%	2.205%
18	15.457	2114	2120	2126	rBB	234064	315888	96.21%	7.657%
19	15.598	2140	2144	2152	rBB	63496	85595	26.07%	2.075%
20	15.692	2157	2160	2163	rBB	1052	1310	0.40%	0.032%
21	17.204	2411	2417	2423	rBV	161825	211706	64.48%	5.132%
22	17.304	2428	2434	2441	rBV2	233572	317023	96.55%	7.685%
23	17.421	2451	2454	2457	rBB	233	337	0.10%	0.008%
24	18.086	2563	2567	2572	rBV3	1179	1422	0.43%	0.034%
25	18.503	2635	2638	2640	rBV	322	347	0.11%	0.008%
26	18.615	2654	2657	2659	rBV	365	406	0.12%	0.010%
27	18.715	2672	2674	2678	rVB2	404	544	0.17%	0.013%
28	18.815	2689	2691	2692	rBV	373	362	0.11%	0.009%
29	19.015	2723	2725	2729	rBV2	380	478	0.15%	0.012%
30	19.080	2734	2736	2739	rVB2	422	507	0.15%	0.012%
31	19.109	2739	2741	2742	rBV	479	378	0.12%	0.009%
32	19.150	2745	2748	2749	rBV2	300	395	0.12%	0.010%
33	19.221	2757	2760	2764	rBV4	1512	2200	0.67%	0.053%
34	19.303	2772	2774	2777	rBV3	409	349	0.11%	0.008%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022621\
 Data File : BM028899.D
 Acq On : 25 Feb 2021 16:36
 Operator : CG/JU
 Sample : PB134807BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK07

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
 Title : SVOA CALIBRATION

35	19.374	2784	2786	2789	rVB	867	638	0.19%	0.015%
36	19.474	2800	2803	2806	rBV2	1180	1494	0.46%	0.036%
37	19.509	2808	2809	2812	rBV2	447	521	0.16%	0.013%
38	19.550	2814	2816	2817	rBV2	583	533	0.16%	0.013%
39	19.586	2817	2822	2829	rVV	242665	325497	99.13%	7.890%
40	19.656	2833	2834	2835	rBV2	710	434	0.13%	0.011%
41	19.792	2855	2857	2860	rBV2	840	1214	0.37%	0.029%
42	19.821	2860	2862	2866	rVB3	832	1252	0.38%	0.030%
43	19.856	2866	2868	2871	rBV4	525	622	0.19%	0.015%
44	19.992	2890	2891	2894	rBV3	917	851	0.26%	0.021%
45	20.062	2901	2903	2904	rBV	791	542	0.17%	0.013%
46	20.303	2942	2944	2946	rBV2	981	613	0.19%	0.015%
47	21.362	3120	3124	3130	rBV	159835	195909	59.67%	4.749%
48	23.438	3470	3477	3484	rVB	184882	328344	100.00%	7.959%
49	23.574	3494	3500	3510	rVB2	111827	204474	62.27%	4.957%


Sum of corrected areas: 4125225

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022621\
Data File : BM028899.D
Acq On : 25 Feb 2021 16:36
Operator : CG/JU
Sample : PB134807BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK07

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

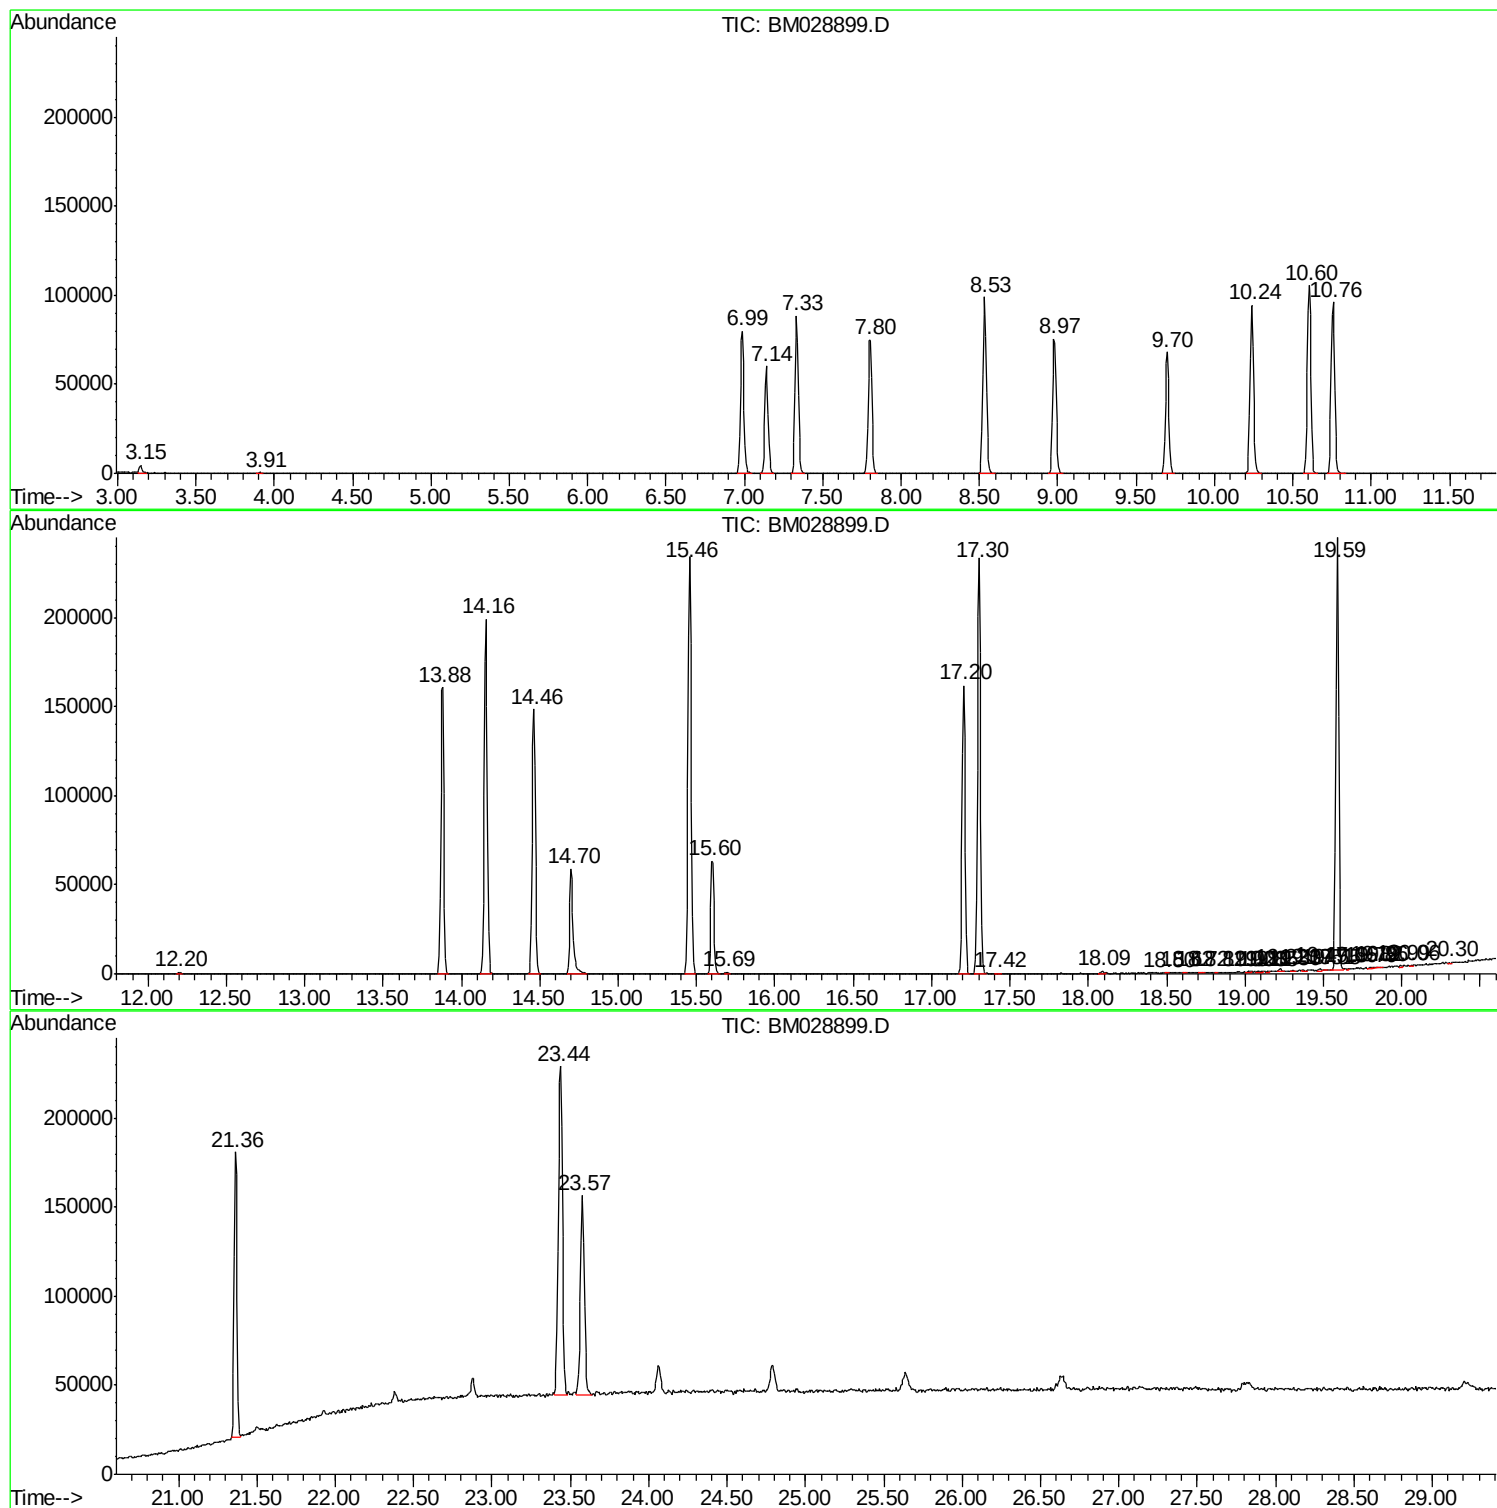

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022621\
Data File : BM028899.D
Acq On : 25 Feb 2021 16:36
Operator : CG/JU
Sample : PB134807BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK07

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022621\
Data File : BM028899.D
Acq On : 25 Feb 2021 16:36
Operator : CG/JU
Sample : PB134807BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK07

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc