

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022621\
 Data File : BM028900.D
 Acq On : 25 Feb 2021 17:13
 Operator : CG/JU
 Sample : M1453-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.046	8	10	12	rVB	236	213	0.13%	0.026%
2	3.075	12	15	18	rBB	203	329	0.19%	0.040%
3	3.099	18	19	21	rBV	195	193	0.11%	0.023%
4	3.146	25	27	29	rBB	198	199	0.12%	0.024%
5	3.910	154	157	159	rBB	449	357	0.21%	0.043%
6	7.798	813	818	826	rBB	46873	72640	42.85%	8.836%
7	10.604	1288	1295	1304	rBB	64178	103537	61.08%	12.594%
8	14.463	1945	1951	1958	rBB2	102491	143779	84.82%	17.489%
9	16.992	2380	2381	2383	rBB2	345	211	0.12%	0.026%
10	17.109	2399	2401	2402	rBV	199	192	0.11%	0.023%
11	17.162	2406	2410	2411	rBV	195	250	0.15%	0.030%
12	17.203	2411	2417	2427	rVV	127451	169504	100.00%	20.618%
13	17.298	2430	2433	2437	rVB2	364	474	0.28%	0.058%
14	17.398	2447	2450	2454	rBV	228	485	0.29%	0.059%
15	18.092	2565	2568	2572	rBV	486	674	0.40%	0.082%
16	18.162	2578	2580	2582	rVB	239	205	0.12%	0.025%
17	18.186	2582	2584	2585	rBV	308	181	0.11%	0.022%
18	18.339	2607	2610	2612	rBV	359	208	0.12%	0.025%
19	18.403	2619	2621	2624	rBB	280	266	0.16%	0.032%
20	18.456	2624	2630	2632	rBV	261	362	0.21%	0.044%
21	18.539	2641	2644	2645	rBV	223	186	0.11%	0.023%
22	18.568	2648	2649	2652	rVB	237	213	0.13%	0.026%
23	18.598	2652	2654	2656	rBV	231	184	0.11%	0.022%
24	18.633	2659	2660	2663	rBV	440	311	0.18%	0.038%
25	18.721	2671	2675	2677	rBV	286	367	0.22%	0.045%
26	18.739	2677	2678	2680	rBV	242	204	0.12%	0.025%
27	18.774	2682	2684	2685	rBV	614	349	0.21%	0.042%
28	18.798	2685	2688	2690	rVB	385	335	0.20%	0.041%
29	18.815	2690	2691	2692	rBV	368	201	0.12%	0.024%
30	18.898	2701	2705	2707	rBV2	322	389	0.23%	0.047%
31	18.921	2707	2709	2710	rVB2	387	215	0.13%	0.026%
32	18.956	2710	2715	2718	rBV2	418	669	0.39%	0.081%
33	18.986	2718	2720	2724	rVB2	358	367	0.22%	0.045%
34	19.021	2724	2726	2727	rVB2	428	292	0.17%	0.036%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022621\
 Data File : BM028900.D
 Acq On : 25 Feb 2021 17:13
 Operator : CG/JU
 Sample : M1453-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
 Title : SVOA CALIBRATION

35	19.033	2727	2728	2729	rBV	783	406	0.24%	0.049%
36	19.050	2729	2731	2733	rBV	252	214	0.13%	0.026%
37	19.133	2743	2745	2747	rBV	365	297	0.18%	0.036%
38	19.156	2747	2749	2751	rVV3	375	305	0.18%	0.037%
39	19.174	2751	2752	2753	rVB	488	172	0.10%	0.021%
40	19.197	2755	2756	2757	rBV	394	246	0.15%	0.030%
41	19.239	2761	2763	2765	rVV	330	256	0.15%	0.031%
42	19.286	2767	2771	2773	rVB2	404	473	0.28%	0.058%
43	19.380	2785	2787	2789	rBV3	407	347	0.20%	0.042%
44	19.433	2794	2796	2799	rBV3	506	617	0.36%	0.075%
45	19.468	2801	2802	2804	rBV	450	382	0.23%	0.046%
46	19.521	2809	2811	2813	rVV	431	281	0.17%	0.034%
47	19.627	2827	2829	2830	rBV2	484	418	0.25%	0.051%
48	19.668	2835	2836	2840	rVV3	680	749	0.44%	0.091%
49	19.697	2840	2841	2842	rVB	757	274	0.16%	0.033%
50	19.715	2842	2844	2845	rVB2	545	358	0.21%	0.044%
51	19.739	2845	2848	2850	rBV3	570	585	0.35%	0.071%
52	19.756	2850	2851	2853	rBV2	581	538	0.32%	0.065%
53	19.780	2853	2855	2856	rVV2	482	283	0.17%	0.034%
54	19.845	2864	2866	2869	rBV2	777	801	0.47%	0.097%
55	19.921	2878	2879	2880	rBV	800	369	0.22%	0.045%
56	20.215	2927	2929	2932	rBV3	784	976	0.58%	0.119%
57	21.362	3120	3124	3129	rBV	137043	164749	97.19%	20.040%
58	23.574	3495	3500	3506	rVB	87293	149460	88.17%	18.180%


Sum of corrected areas: 822097

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM022621\
Data File : BM028900.D
Acq On : 25 Feb 2021 17:13
Operator : CG/JU
Sample : M1453-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

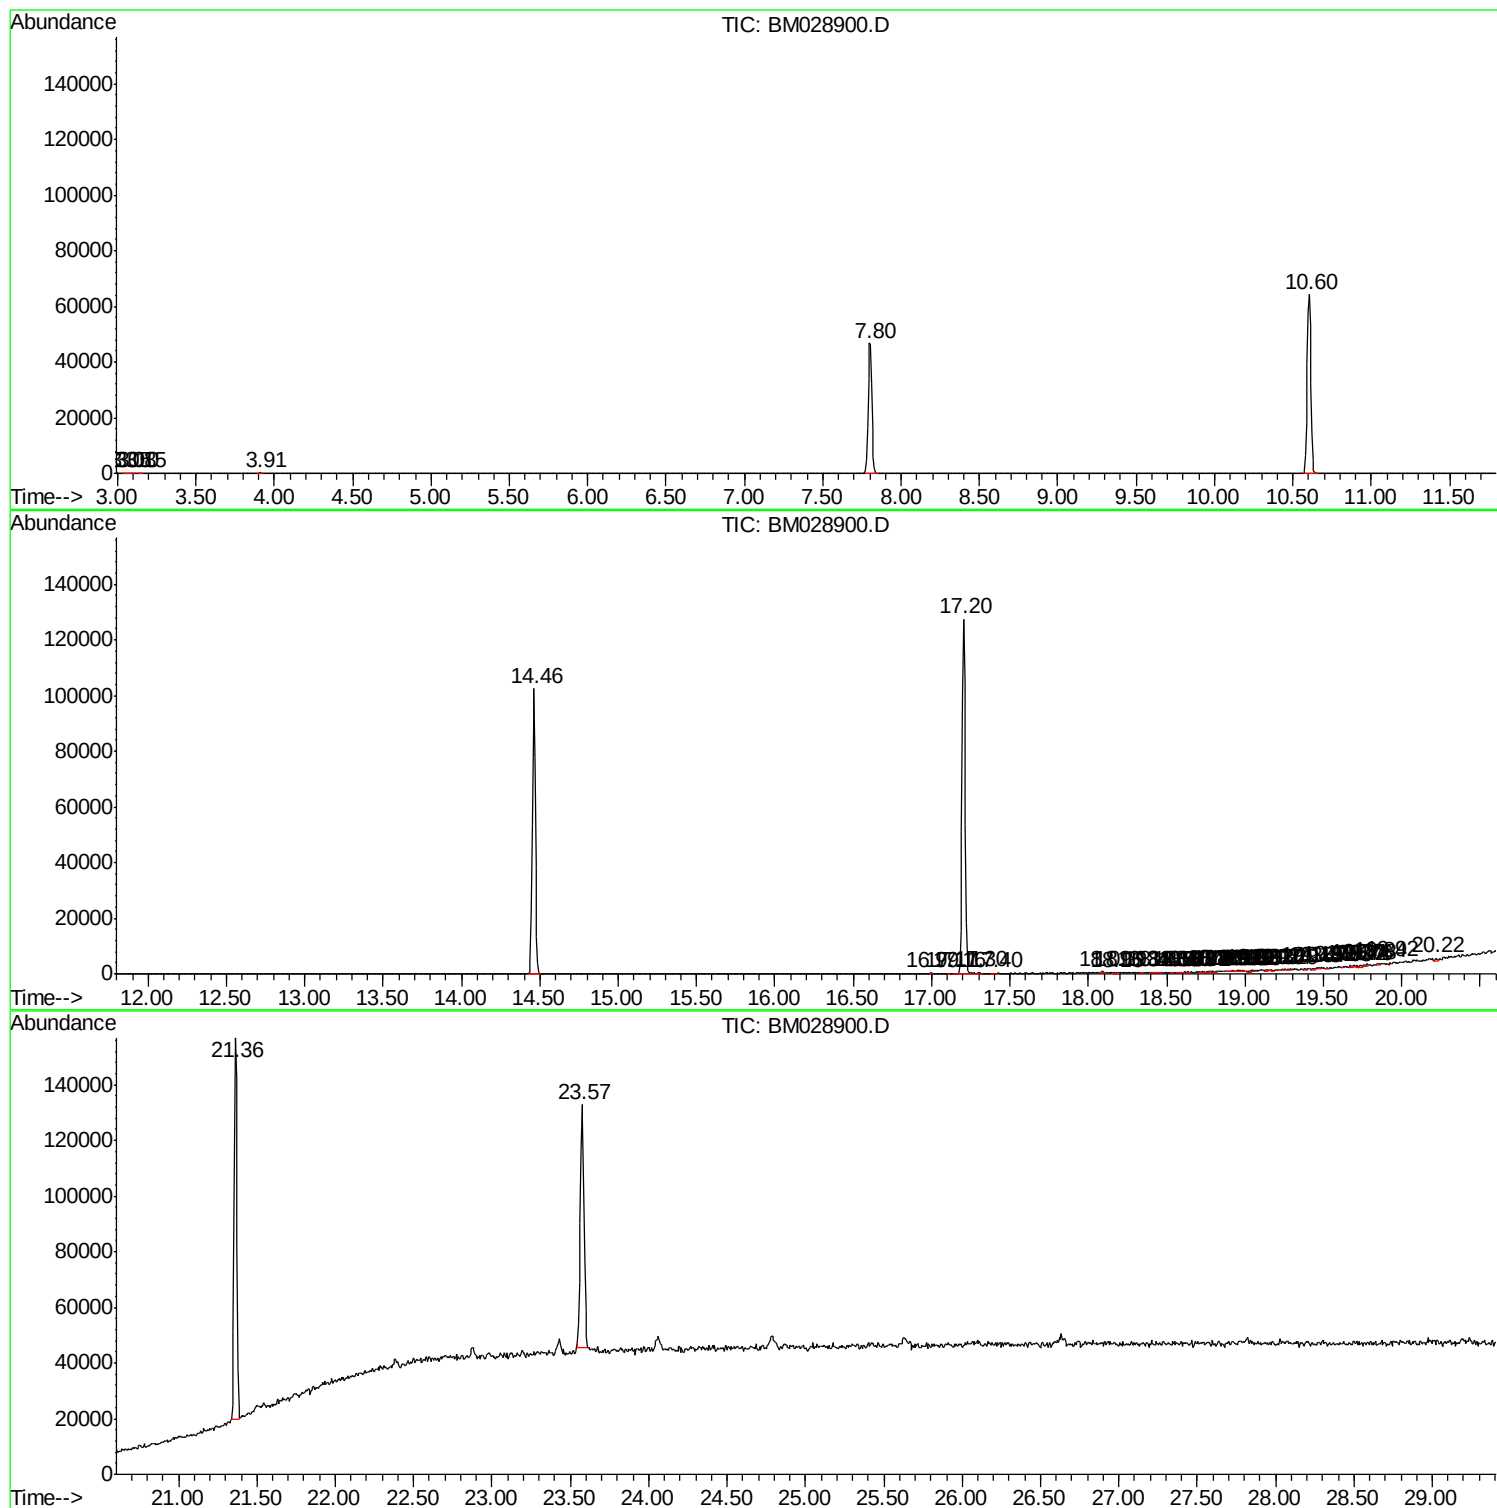

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022621\
Data File : BM028900.D
Acq On : 25 Feb 2021 17:13
Operator : CG/JU
Sample : M1453-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM022621\
Data File : BM028900.D
Acq On : 25 Feb 2021 17:13
Operator : CG/JU
Sample : M1453-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc