


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM022621\
 Data File : BM028896.D
 Acq On : 25 Feb 2021 14:06
 Operator : CG/JU
 Sample : DFTPP36
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP36

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022121MA.M
 Title : SVOA CALIBRATION
 Last Update : Thu Feb 25 15:24:23 2021

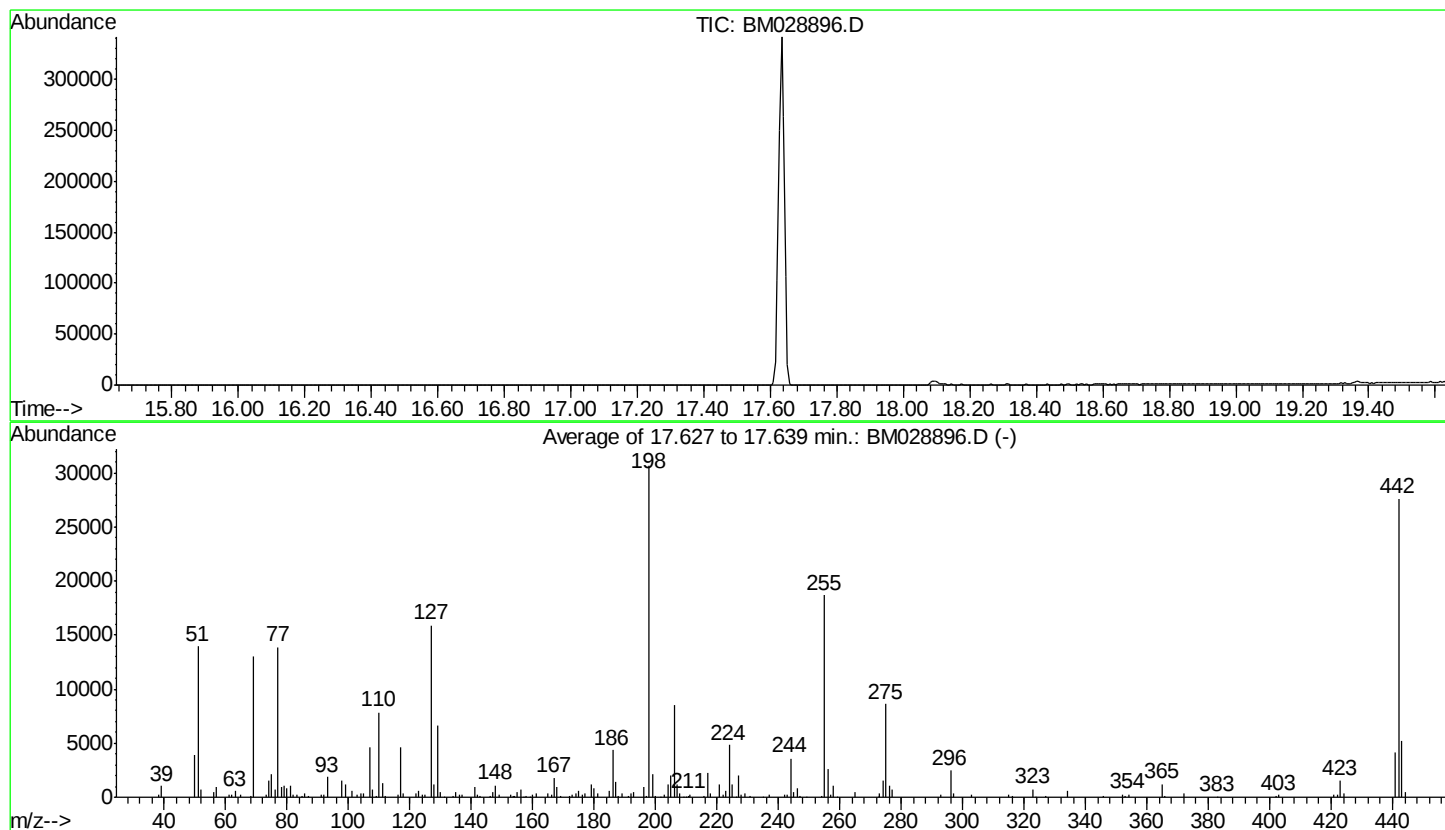

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	13960	PASS
68	69	0.00	2	1.1	145	PASS
69	198	0.00	100	42.3	12990	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	15913	PASS
197	198	0.00	2	0.3	86	PASS
198	198	100	100	100.0	30688	PASS
199	198	5	9	6.9	2131	PASS
275	198	10	60	28.0	8607	PASS
365	198	1	100	4.0	1231	PASS
441	198	0.01	100	13.6	4186	PASS
442	198	50	100	90.0	27626	PASS
443	442	15	24	19.1	5267	PASS

Scan 2484 (17.598 min): BM028896.D
DFTPP36

m/z	Abundance
43.90	161.0
207.00	257.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

m/z	Abundance
38.00	197.0
39.00	1077.0
50.10	3792.0
51.00	14294.0
52.00	791.0
56.00	456.0
57.00	914.0
60.90	193.0
62.10	168.0
63.00	501.0
65.00	245.0
68.10	251.0
69.00	13023.0
73.00	236.0
74.00	1543.0
75.00	2031.0
76.00	763.0
77.00	13655.0
78.00	1031.0
79.00	1012.0
80.00	727.0
81.00	1050.0
82.00	229.0
83.00	224.0
84.90	150.0
85.90	300.0
91.00	246.0
92.00	341.0
93.00	1915.0
98.00	1576.0
99.00	1112.0
101.00	622.0
102.90	194.0
104.00	394.0
105.00	350.0
107.00	4446.0
108.00	721.0
110.00	7673.0
111.00	1292.0
111.90	195.0
116.00	305.0
117.00	4570.0
117.90	331.0
122.00	414.0
122.90	531.0
123.80	254.0
125.00	159.0
127.00	14816.0
128.00	1058.0
129.00	6370.0
130.00	525.0
133.90	166.0
135.00	478.0
136.00	180.0
136.90	253.0
141.00	843.0
142.00	224.0
142.90	174.0
146.00	154.0
146.90	471.0
147.90	1066.0
148.90	186.0
152.90	239.0
153.80	212.0
155.00	455.0
156.00	681.0
160.00	244.0
161.00	375.0
164.90	333.0
166.00	205.0
167.00	1656.0
168.00	981.0
168.90	181.0
173.00	164.0
174.00	340.0
174.90	515.0
176.00	169.0
176.90	263.0
178.90	1135.0
180.00	770.0
180.90	423.0
185.00	497.0
186.00	3853.0
187.00	1184.0
188.90	323.0
191.00	191.0
191.90	368.0
193.00	466.0
195.90	929.0
197.90	27048.0
198.90	1902.0
203.00	174.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

204.00	1127.0
205.00	1789.0
206.00	7505.0
207.00	1224.0
208.00	305.0
210.90	300.0
217.00	2078.0
218.00	283.0
220.90	1034.0
221.90	318.0
223.00	520.0
224.00	4219.0
225.00	1113.0
227.00	1868.0
227.90	207.0
228.90	311.0
231.00	189.0
237.00	159.0
242.00	259.0
243.00	227.0
244.00	2954.0
245.00	484.0
246.00	734.0
254.20	197.0
255.00	15422.0
256.00	2307.0
257.00	184.0
258.00	893.0
265.00	381.0
272.80	333.0
274.00	1035.0
275.00	6972.0
276.00	791.0
276.90	617.0
292.90	205.0
296.00	1839.0
297.00	258.0
303.00	230.0
314.90	185.0
323.00	543.0
334.00	477.0
352.00	185.0
352.90	157.0
354.10	205.0
365.00	934.0
372.00	287.0
402.90	167.0
422.00	162.0
423.00	984.0
424.00	392.0
441.00	2689.0
442.00	18240.0
443.00	3631.0
444.00	306.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

m/z	Abundance
38.00	262.0
39.00	1182.0
50.10	4709.0
51.10	16736.0
52.00	808.0
55.90	515.0
57.00	1130.0
61.00	211.0
62.00	227.0
63.00	669.0
65.00	264.0
69.00	15691.0
73.00	376.0
74.00	1919.0
75.00	2637.0
76.00	836.0
77.00	16632.0
78.00	1267.0
79.00	1273.0
80.00	1005.0
81.00	1297.0
82.00	310.0
83.00	295.0
85.00	220.0
85.90	475.0
86.90	221.0
90.90	266.0
92.00	290.0
93.00	2098.0
98.00	1839.0
99.00	1302.0
101.00	640.0
103.00	227.0
104.00	487.0
105.00	478.0
107.00	5527.0
108.00	889.0
109.00	193.0
110.00	9333.0
111.00	1507.0
111.90	188.0
115.90	350.0
117.00	5245.0
117.90	393.0
122.00	360.0
123.00	636.0
123.90	244.0
125.00	225.0
127.00	19168.0
127.90	1424.0
129.00	7803.0
130.00	632.0
131.00	152.0
133.00	225.0
133.90	225.0
135.00	646.0
135.90	257.0
137.00	328.0
141.00	1077.0
141.90	266.0
142.90	207.0
145.90	206.0
147.00	570.0
147.90	1296.0
148.90	344.0
152.90	404.0
154.00	215.0
155.00	583.0
156.00	855.0
156.90	162.0
157.90	178.0
158.90	152.0
159.90	337.0
161.00	444.0
165.00	430.0
165.90	313.0
167.00	2177.0
168.00	1010.0
169.00	199.0
172.00	191.0
172.90	253.0
174.00	394.0
175.00	698.0
175.90	233.0
177.00	378.0
178.90	1447.0
180.00	1081.0
180.90	470.0
185.00	778.0
186.00	5239.0
187.00	1740.0
188.00	212.0
188.90	400.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

190.90	182.0
191.90	463.0
192.90	590.0
196.00	1095.0
197.00	258.0
198.00	36720.0
198.90	2627.0
200.00	200.0
201.40	175.0
203.00	253.0
204.00	1503.0
205.00	2376.0
206.00	10214.0
207.00	1676.0
208.00	397.0
209.00	153.0
210.10	168.0
211.10	441.0
216.00	246.0
217.00	2640.0
218.00	425.0
221.00	1363.0
222.00	369.0
222.90	656.0
224.00	5717.0
225.00	1307.0
226.00	167.0
227.00	2359.0
227.90	372.0
228.90	426.0
230.90	187.0
234.90	166.0
236.90	220.0
241.90	335.0
243.00	263.0
244.00	4224.0
245.00	633.0
246.00	918.0
246.90	239.0
248.90	169.0
254.10	291.0
255.00	22056.0
256.00	3125.0
257.00	256.0
258.00	1414.0
258.90	173.0
264.90	497.0
273.00	550.0
274.00	1867.0
275.00	10287.0
276.00	1484.0
276.90	889.0
293.00	223.0
296.00	2924.0
296.90	405.0
303.00	238.0
314.90	360.0
316.00	189.0
323.00	899.0
323.90	164.0
326.90	197.0
334.00	631.0
346.00	168.0
352.00	242.0
353.90	276.0
365.00	1379.0
366.00	198.0
372.00	478.0
383.00	182.0
402.00	223.0
402.90	224.0
421.00	277.0
422.00	271.0
423.00	1817.0
423.90	450.0
441.00	4866.0
442.00	32440.0
443.00	6186.0
444.00	595.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

m/z	Abundance
38.00	174.0
39.10	923.0
50.00	3081.0
51.10	10851.0
52.00	596.0
56.00	304.0
57.00	770.0
61.00	155.0
61.90	159.0
63.00	497.0
65.10	188.0
68.10	185.0
69.00	10256.0
73.00	221.0
74.00	1186.0
75.00	1697.0
76.10	619.0
77.10	11349.0
78.10	708.0
79.00	872.0
79.90	714.0
81.00	780.0
81.90	237.0
83.00	198.0
84.90	161.0
85.90	238.0
90.90	214.0
91.90	226.0
93.00	1601.0
98.00	1248.0
98.90	1006.0
100.90	434.0
102.90	186.0
103.90	334.0
104.90	333.0
107.00	4017.0
108.00	488.0
110.00	6629.0
111.00	1009.0
115.90	241.0
117.00	3886.0
118.00	263.0
122.00	351.0
122.90	494.0
123.90	204.0
124.90	185.0
127.00	13756.0
128.00	1042.0
129.00	5841.0
130.00	436.0
134.00	153.0
134.90	432.0
135.90	162.0
136.90	255.0
140.90	861.0
141.90	255.0
145.90	153.0
147.00	420.0
148.00	897.0
148.90	197.0
153.00	255.0
153.90	183.0
155.00	442.0
156.00	573.0
158.00	172.0
159.90	235.0
160.90	379.0
164.90	322.0
165.90	155.0
167.00	1583.0
168.00	752.0
168.90	161.0
171.90	183.0
173.00	193.0
173.90	351.0
175.00	602.0
175.90	190.0
177.00	298.0
178.90	1090.0
180.00	712.0
181.00	335.0
185.00	621.0
186.00	3963.0
187.00	1250.0
188.90	304.0
191.90	407.0
193.00	424.0
195.90	943.0
198.00	28296.0
198.90	1865.0
202.90	227.0
204.00	1068.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

205.00	1828.0
206.00	7874.0
207.00	1274.0
207.90	298.0
211.00	335.0
215.90	154.0
216.90	2150.0
218.00	330.0
220.90	1134.0
222.90	479.0
224.00	4572.0
225.00	1100.0
227.00	1926.0
228.00	261.0
229.00	414.0
236.90	192.0
242.00	190.0
243.00	212.0
244.00	3506.0
245.00	439.0
246.00	691.0
247.00	151.0
255.00	18592.0
256.00	2494.0
256.90	183.0
258.00	1030.0
264.90	510.0
272.90	580.0
274.00	1555.0
275.00	8563.0
276.00	1087.0
276.90	699.0
292.90	197.0
296.00	2678.0
297.00	431.0
303.00	267.0
314.90	266.0
323.00	712.0
334.00	551.0
345.90	197.0
351.90	269.0
353.00	166.0
354.00	285.0
365.00	1380.0
372.00	470.0
401.90	260.0
402.90	268.0
420.90	278.0
422.00	201.0
423.00	1694.0
424.00	387.0
441.00	5004.0
442.00	32200.0
443.00	5986.0
444.00	573.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36