


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM030421\
 Data File : BM028979.D
 Acq On : 04 Mar 2021 08:30
 Operator : CG/JU
 Sample : DFTPP40
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP40

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM022721MA.M
 Title : SVOA CALIBRATION
 Last Update : Thu Mar 04 09:45:23 2021

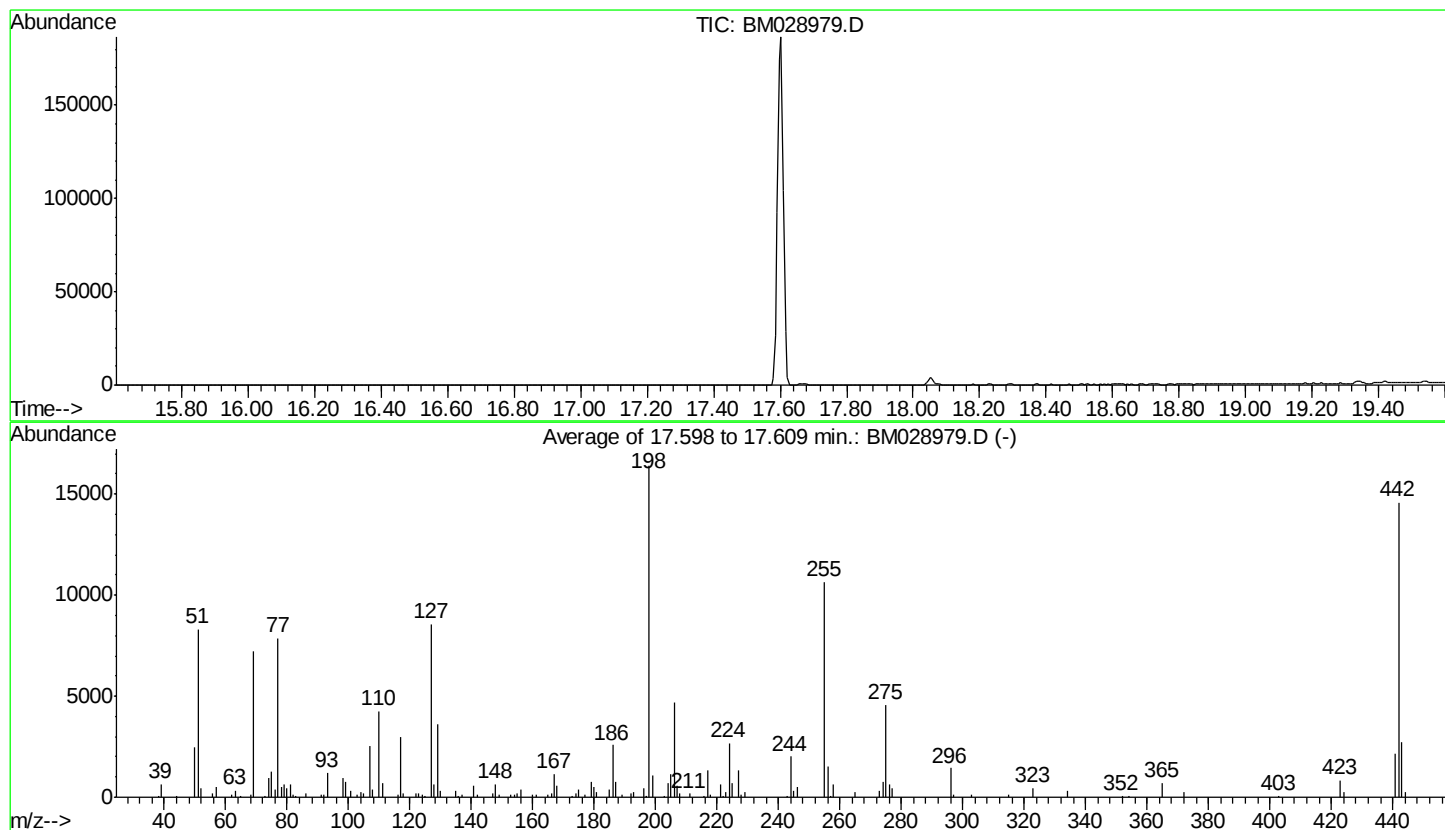

AutoFind: Scans 2484, 2485, 2486; Background Corrected with Scan 2479

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.7	8311	PASS
68	69	0.00	2	1.6	117	PASS
69	198	0.00	100	43.8	7194	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.2	8566	PASS
197	198	0.00	2	0.3	51	PASS
198	198	100	100	100.0	16408	PASS
199	198	5	9	6.5	1063	PASS
275	198	10	60	27.8	4561	PASS
365	198	1	100	4.3	713	PASS
441	198	0.01	100	13.2	2170	PASS
442	198	50	100	88.9	14593	PASS
443	442	15	24	18.8	2745	PASS

Scan 2479 (17.568 min): BM028979.D
DFTPP40

m/z	Abundance
206.90	152.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

m/z	Abundance
38.00	159.0
39.00	838.0
50.00	3054.0
51.10	10669.0
52.00	432.0
55.90	333.0
57.00	613.0
62.00	167.0
63.00	447.0
68.10	166.0
69.00	8951.0
72.90	157.0
74.00	1160.0
75.00	1592.0
76.00	469.0
77.10	9817.0
78.00	672.0
79.00	810.0
80.00	531.0
81.00	809.0
82.00	153.0
82.90	176.0
85.90	309.0
91.00	168.0
92.00	200.0
93.00	1494.0
98.00	1271.0
99.00	941.0
100.90	396.0
102.90	150.0
104.00	322.0
105.00	316.0
107.00	2881.0
108.00	460.0
110.00	5119.0
111.00	842.0
115.90	154.0
117.00	3596.0
117.90	269.0
122.00	229.0
122.90	355.0
124.00	168.0
127.00	10418.0
127.90	826.0
129.00	4176.0
130.00	389.0
134.90	338.0
135.90	158.0
137.00	197.0
140.90	621.0
142.00	155.0
147.00	324.0
147.90	771.0
148.90	171.0
152.90	169.0
153.90	169.0
154.90	314.0
156.00	447.0
159.90	231.0
161.00	254.0
164.90	195.0
166.00	154.0
167.00	1436.0
168.00	666.0
174.00	209.0
175.00	429.0
176.90	278.0
178.90	834.0
179.90	541.0
180.90	266.0
184.90	440.0
186.00	2917.0
187.00	735.0
188.90	233.0
191.90	279.0
193.00	304.0
195.90	534.0
196.80	154.0
197.10	154.0
198.00	18096.0
198.90	1125.0
204.00	769.0
205.00	1191.0
206.00	5125.0
207.00	769.0
207.90	244.0
210.90	195.0
216.90	1596.0
217.90	181.0
221.00	719.0
223.00	330.0
224.00	2818.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

225.00	677.0
227.00	1491.0
227.90	212.0
228.90	292.0
244.00	2157.0
245.00	329.0
245.90	514.0
255.00	11291.0
256.00	1588.0
257.90	646.0
264.90	271.0
273.00	299.0
274.00	820.0
275.00	4733.0
276.00	631.0
277.00	467.0
296.00	1407.0
296.90	172.0
303.00	173.0
314.90	225.0
323.00	442.0
334.00	359.0
365.00	783.0
372.00	223.0
423.00	840.0
423.90	280.0
440.90	1866.0
442.00	12640.0
443.00	2689.0
443.90	254.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

m/z	Abundance
39.00	795.0
44.00	154.0
50.10	2733.0
51.00	9637.0
52.00	554.0
55.90	234.0
57.00	693.0
62.00	167.0
63.00	345.0
65.00	184.0
68.00	186.0
69.00	8317.0
74.00	1105.0
75.00	1500.0
76.00	482.0
77.10	9242.0
78.10	610.0
79.00	764.0
80.00	499.0
81.00	786.0
82.00	163.0
86.00	275.0
90.90	177.0
92.00	216.0
93.00	1451.0
98.00	1086.0
98.90	819.0
100.90	439.0
102.90	156.0
104.00	285.0
104.90	335.0
107.00	3074.0
107.90	481.0
110.00	5057.0
111.00	751.0
116.00	199.0
117.00	3420.0
118.00	231.0
121.90	259.0
122.90	309.0
123.90	174.0
124.90	152.0
127.00	10019.0
128.00	643.0
129.00	4300.0
129.90	372.0
134.90	341.0
137.00	156.0
140.90	767.0
141.90	218.0
147.00	309.0
148.00	791.0
148.90	164.0
152.90	174.0
153.90	155.0
154.90	316.0
156.00	423.0
159.80	160.0
161.00	216.0
164.90	207.0
165.90	237.0
167.00	1305.0
167.90	677.0
172.90	152.0
174.00	301.0
175.00	445.0
176.90	193.0
179.00	923.0
180.00	574.0
180.90	275.0
185.00	434.0
186.00	3197.0
187.00	894.0
188.90	193.0
191.90	265.0
192.90	346.0
196.00	641.0
197.90	19472.0
198.90	1236.0
202.90	162.0
204.00	830.0
205.00	1460.0
206.00	5652.0
207.00	907.0
208.00	292.0
211.00	163.0
215.90	153.0
217.00	1490.0
217.90	189.0
220.90	786.0
221.80	255.0
223.00	332.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

224.00	3414.0
225.00	894.0
227.00	1562.0
227.90	256.0
229.00	286.0
243.00	158.0
244.00	2470.0
245.00	340.0
246.00	587.0
255.00	12705.0
256.00	1864.0
256.90	181.0
257.90	870.0
265.00	354.0
272.90	413.0
273.90	904.0
275.00	5330.0
276.00	775.0
276.90	468.0
296.00	1807.0
297.00	294.0
303.00	219.0
314.90	216.0
323.00	564.0
334.10	335.0
352.00	214.0
354.00	213.0
365.00	715.0
372.00	285.0
402.90	193.0
422.90	1029.0
423.90	361.0
441.00	2516.0
442.00	17752.0
443.00	3117.0
443.90	317.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40

m/z	Abundance
39.00	362.0
50.00	1543.0
51.00	4627.0
52.00	277.0
56.90	283.0
62.90	185.0
69.00	4315.0
74.00	516.0
75.00	681.0
76.00	245.0
77.10	4565.0
78.00	299.0
79.00	357.0
79.90	281.0
81.00	372.0
93.00	724.0
98.00	537.0
99.00	433.0
100.90	181.0
104.00	184.0
107.00	1639.0
108.00	252.0
110.00	2641.0
111.00	420.0
117.00	1989.0
127.00	5261.0
128.00	415.0
129.00	2352.0
129.90	199.0
134.90	241.0
141.00	350.0
148.00	388.0
155.90	251.0
166.00	163.0
167.00	695.0
168.00	355.0
174.90	256.0
178.90	597.0
179.90	324.0
180.90	177.0
185.00	238.0
186.00	1642.0
187.00	583.0
193.00	196.0
195.90	254.0
197.90	11658.0
198.90	828.0
204.00	520.0
205.00	801.0
206.00	3379.0
207.00	581.0
210.90	161.0
216.90	922.0
221.00	452.0
222.90	169.0
224.00	1797.0
225.00	509.0
227.00	914.0
229.00	183.0
244.00	1421.0
244.90	201.0
245.90	339.0
255.00	7976.0
256.00	1036.0
257.90	484.0
265.00	217.0
273.00	279.0
274.00	644.0
275.00	3620.0
276.00	522.0
277.00	385.0
295.90	1105.0
322.90	375.0
334.00	202.0
365.00	641.0
372.00	193.0
423.00	630.0
423.90	213.0
441.00	2129.0
442.00	13387.0
443.00	2430.0
444.00	211.0

Instrument :
BNA_M
ClientSampleId :
DFTPP40