


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030823\
 Data File : BM038926.D
 Acq On : 08 Mar 2023 11:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\BFDDTBREAKDOWN-8270.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 01 16:14:27 2010

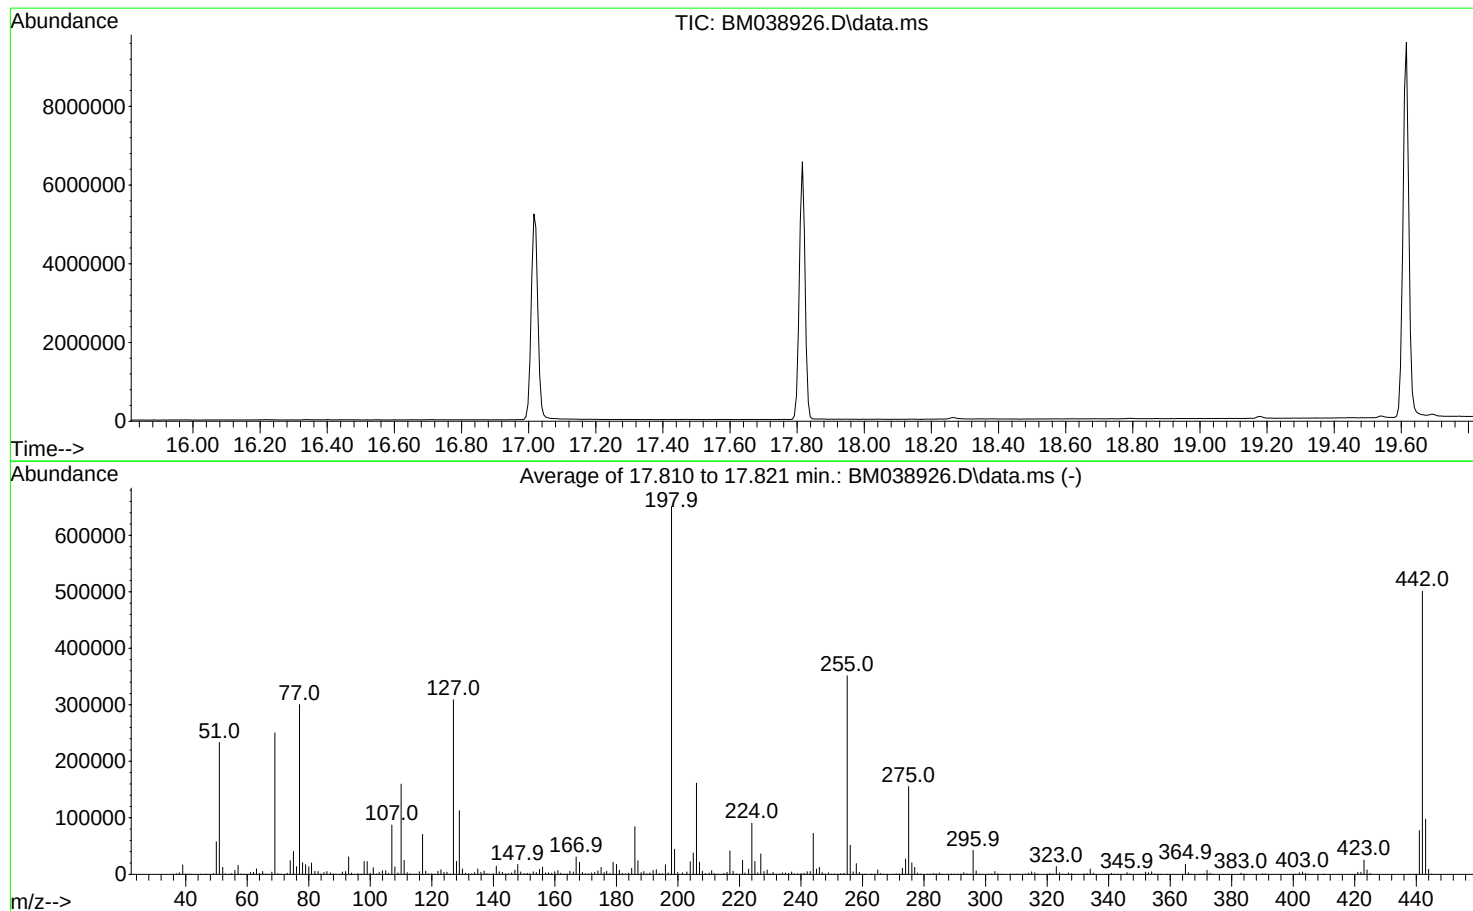




AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	233361	PASS
68	69	0.00	2	1.5	3860	PASS
69	198	0.00	100	38.4	250124	PASS
70	69	0.00	2	0.5	1354	PASS
127	198	10	80	47.4	308864	PASS
197	198	0.00	2	0.4	2431	PASS
198	198	100	100	100.0	651157	PASS
199	198	5	9	6.8	44291	PASS
275	198	10	60	23.8	155264	PASS
365	198	1	100	2.7	17827	PASS
441	442	0.01	24	15.4	77432	PASS
442	198	50	100	77.0	501291	PASS
443	442	15	24	19.4	97451	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030823\
 Data File : BM038926.D
 Acq On : 08 Mar 2023 11:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 09 06:06:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 05:21:24 2023
 Response via : Initial Calibration

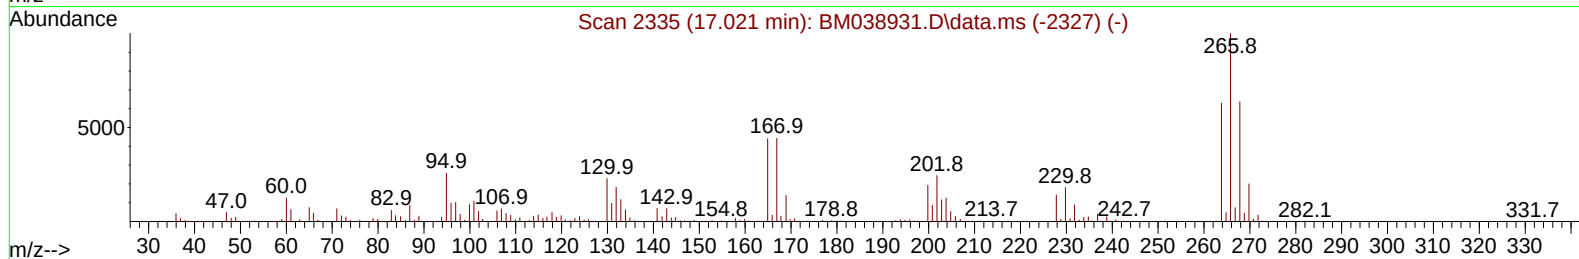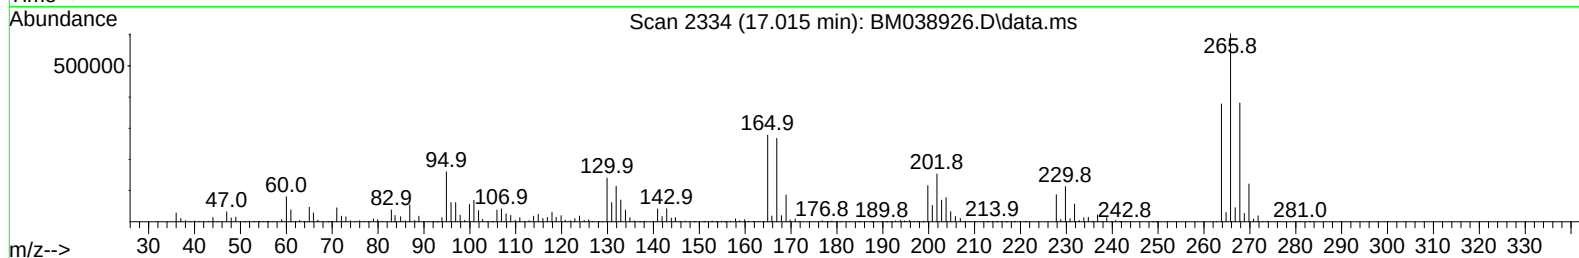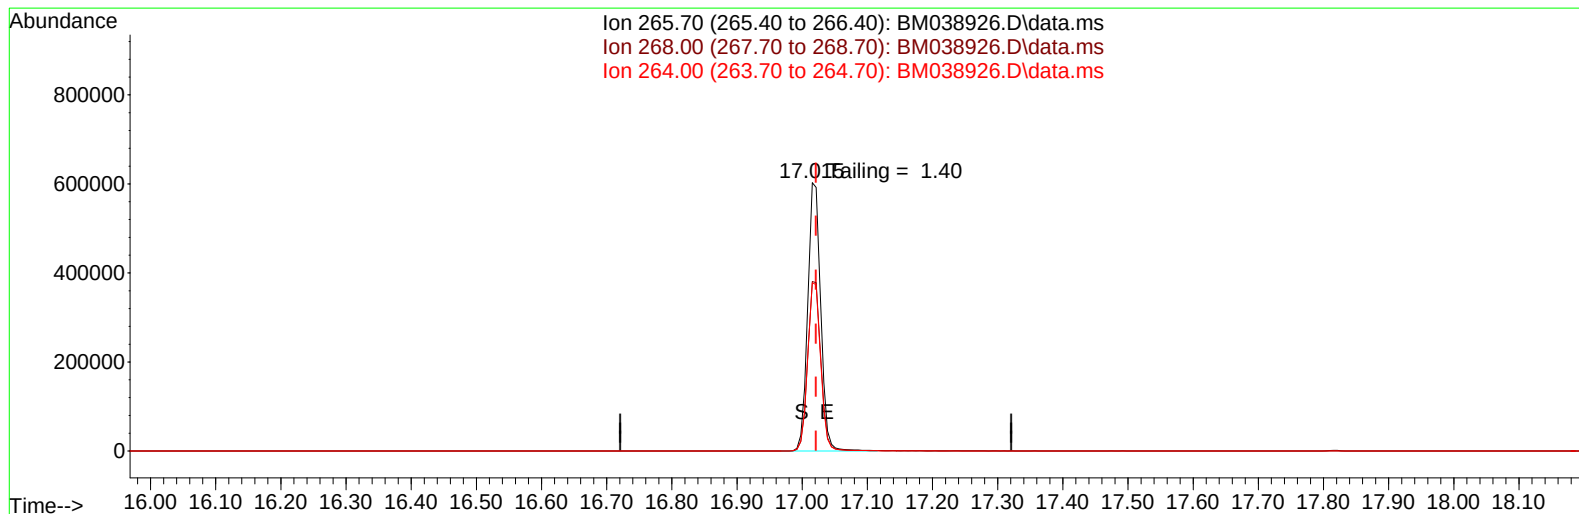

TIC: BM038926.D\data.ms

(70) Pentachlorophenol (C)

17.015min (-0.006) 0.00 ng




response 839081

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.12
264.00	62.90	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM030823\
 Data File : BM038926.D
 Acq On : 08 Mar 2023 11:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 09 06:06:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM030823.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 09 05:21:24 2023
 Response via : Initial Calibration

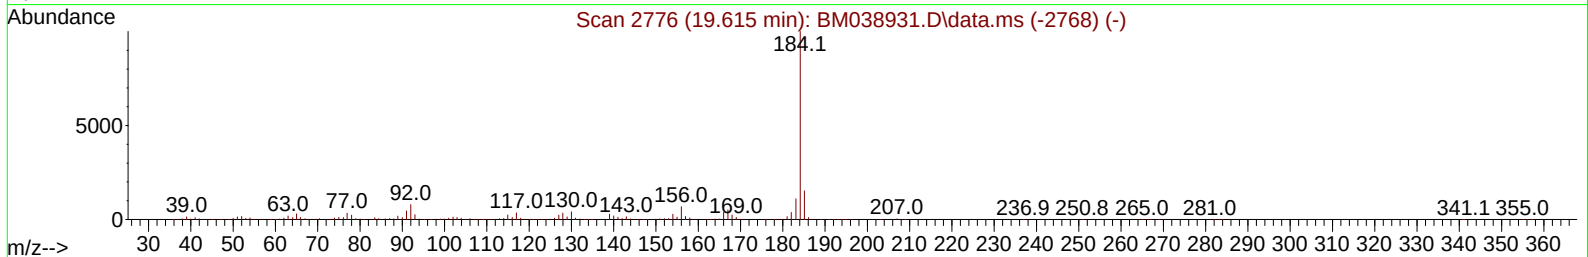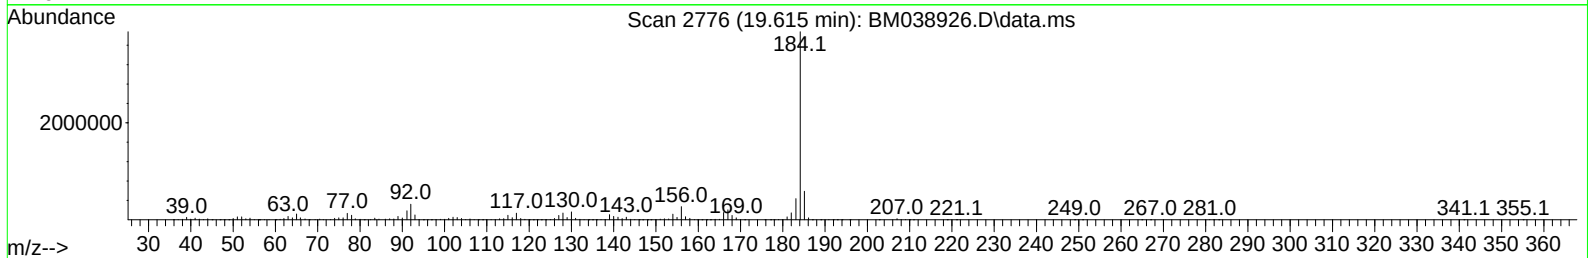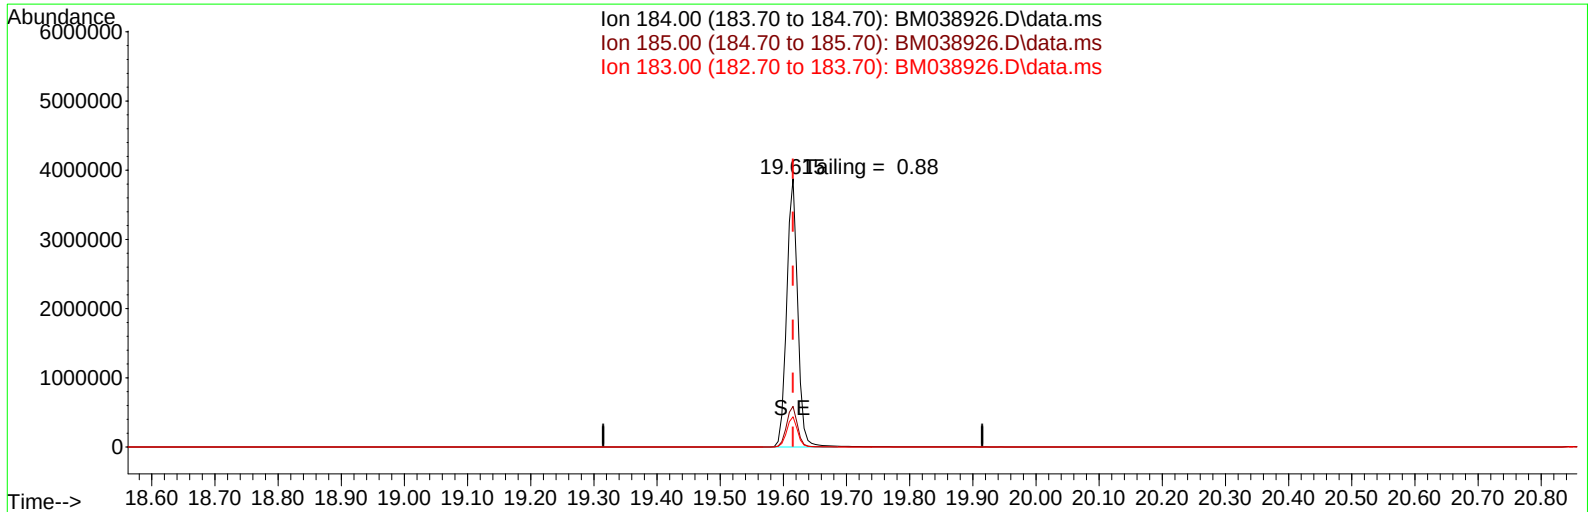

TIC: BM038926.D\data.ms

(77) Benzidine

19.615min (+ 0.000) 3327635.65 ng

response 4727968

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	15.14
183.00	11.00	11.26
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/8/2023	BNA_M	<u>BM038926.D</u>
Compound Name	Response	Retention Time
DDT	2067463	20.85
DDD	13611	20.462
DDE	0	19.868
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13611	2081074	0.65

Instrument :
BNA_M
ClientSampleId :
DFTPP