
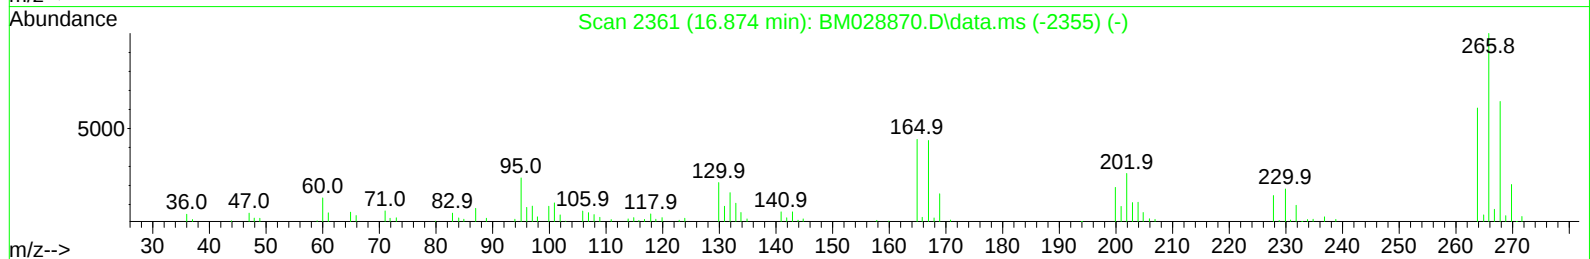
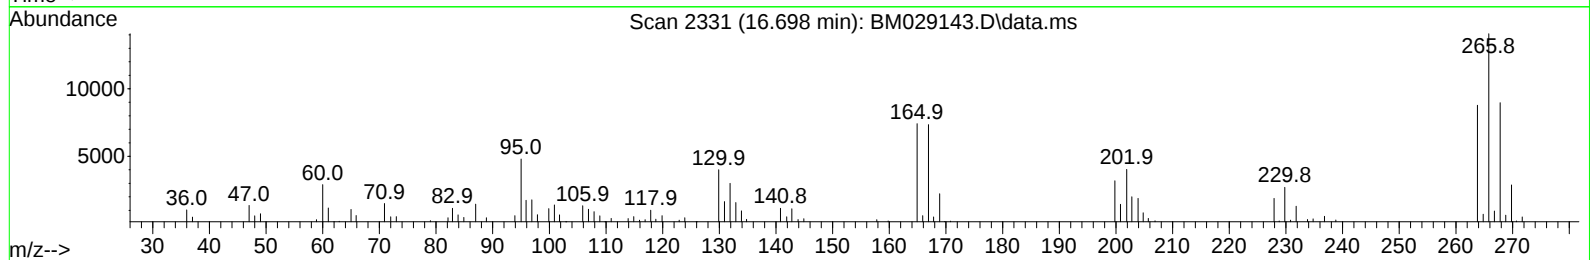


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM31621\
Data File : BM029143.D
Acq On : 16 Mar 2021 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 11:43:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 12 12:30:15 2021
Response via : Initial Calibration

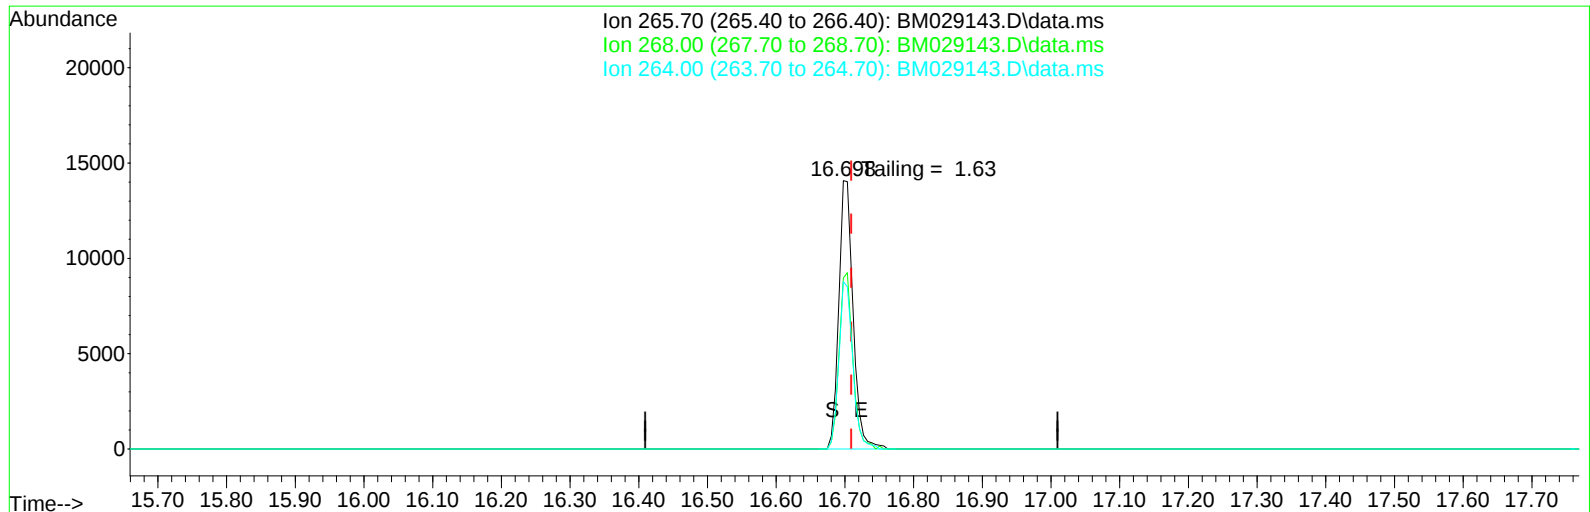

TIC: BM029143.D\data.ms

(70) Pentachlorophenol (C)




16.698min (-0.012) 0.00 ng

response 20352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	63.76
264.00	63.30	62.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM31621\
Data File : BM029143.D
Acq On : 16 Mar 2021 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 11:43:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 12 12:30:15 2021
Response via : Initial Calibration

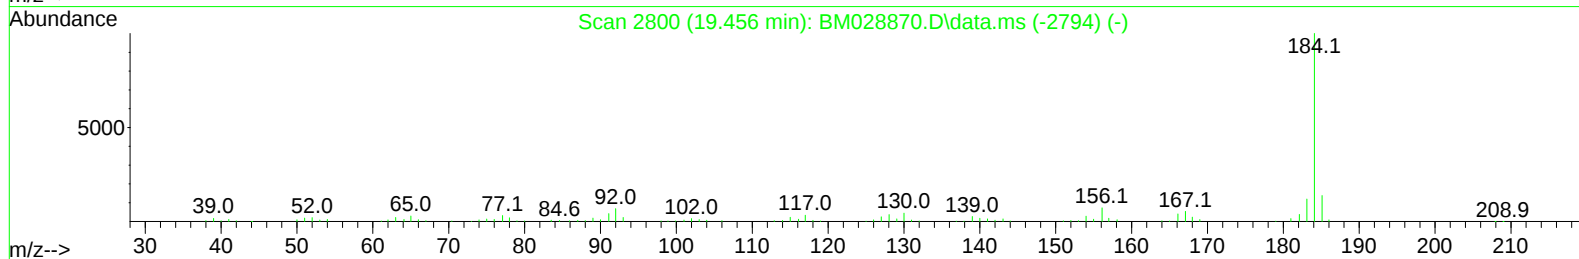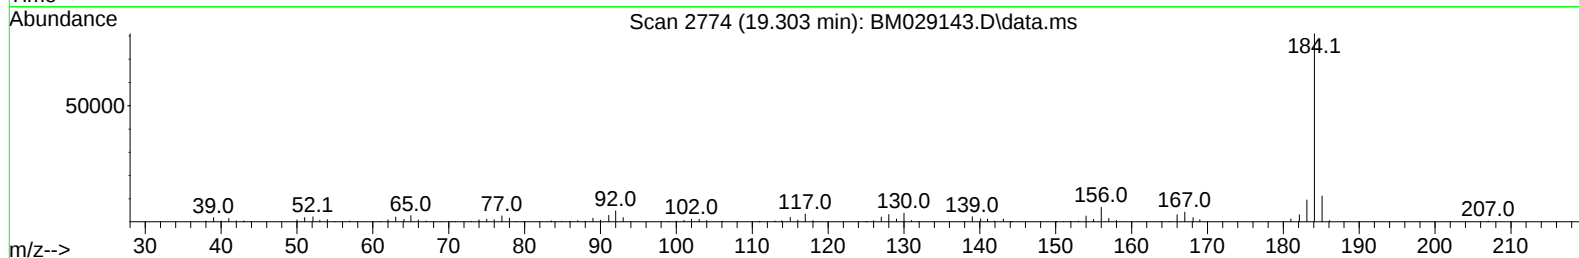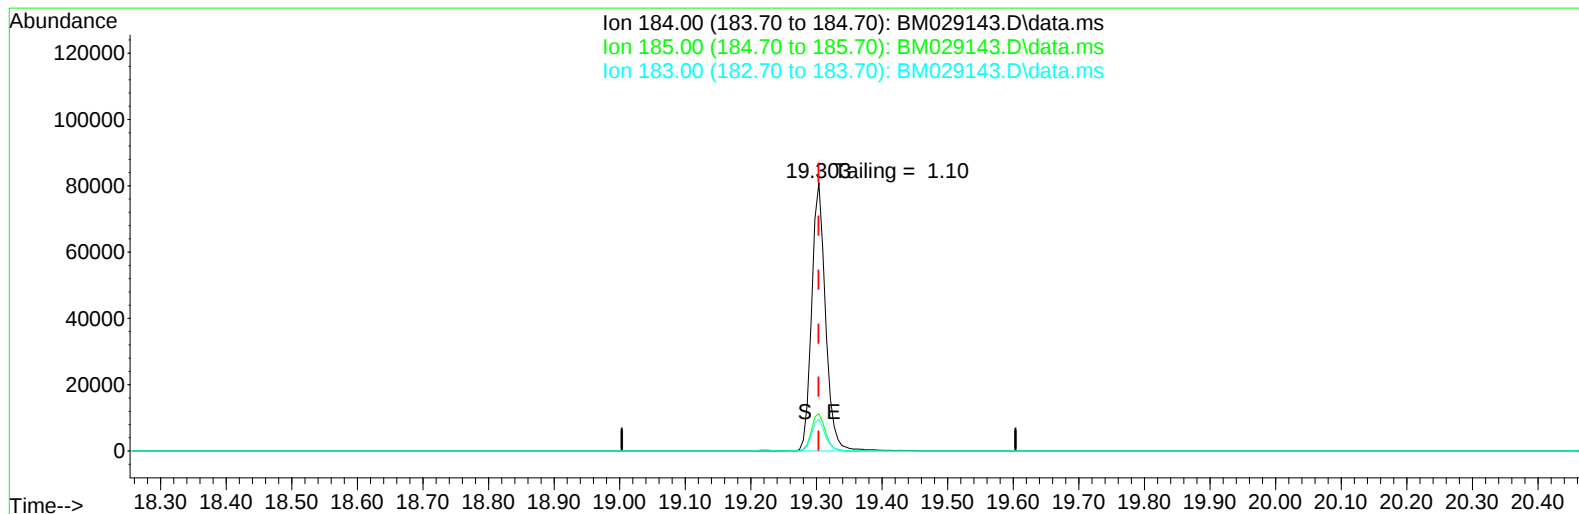

TIC: BM029143.D\data.ms

(77) Benzidine

19.303min (+ 0.000) 0.00 ng

response 119158

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	13.91
183.00	12.10	11.76
0.00	0.00	0.00