

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031621\
 Data File : BM029145.D
 Acq On : 16 Mar 2021 12:14
 Operator : CG/JU
 Sample : PB135177BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135177BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.204	372	377	392	rBV	253419	347506	57.05%	12.029%
2	6.834	647	654	674	rBB	229147	351213	57.65%	12.158%
3	7.610	781	786	794	rBB	42237	63534	10.43%	2.199%
4	8.792	980	987	1000	rBB	138756	219395	36.02%	7.595%
5	10.404	1255	1261	1269	rBB	51000	82372	13.52%	2.851%
6	12.898	1678	1685	1695	rBV	331503	460458	75.59%	15.939%
7	14.286	1915	1921	1927	rBB	73609	102237	16.78%	3.539%
8	15.792	2171	2177	2186	rBB	251909	333947	54.82%	11.560%
9	17.033	2383	2388	2396	rBB	83872	113756	18.67%	3.938%
10	19.668	2830	2836	2840	rBV	539443	609175	100.00%	21.087%
11	21.215	3095	3099	3104	rBV	91747	103498	16.99%	3.583%
12	23.356	3457	3463	3471	rVB2	59345	101719	16.70%	3.521%




Sum of corrected areas: 2888810

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031621\
Data File : BM029145.D
Acq On : 16 Mar 2021 12:14
Operator : CG/JU
Sample : PB135177BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135177BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

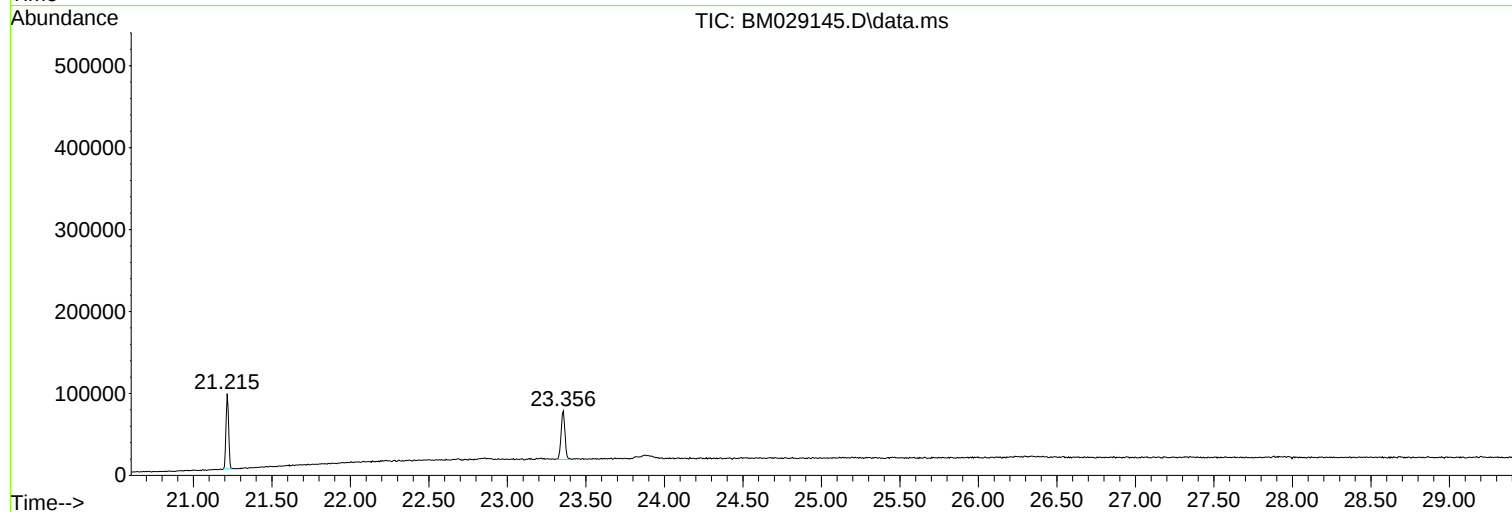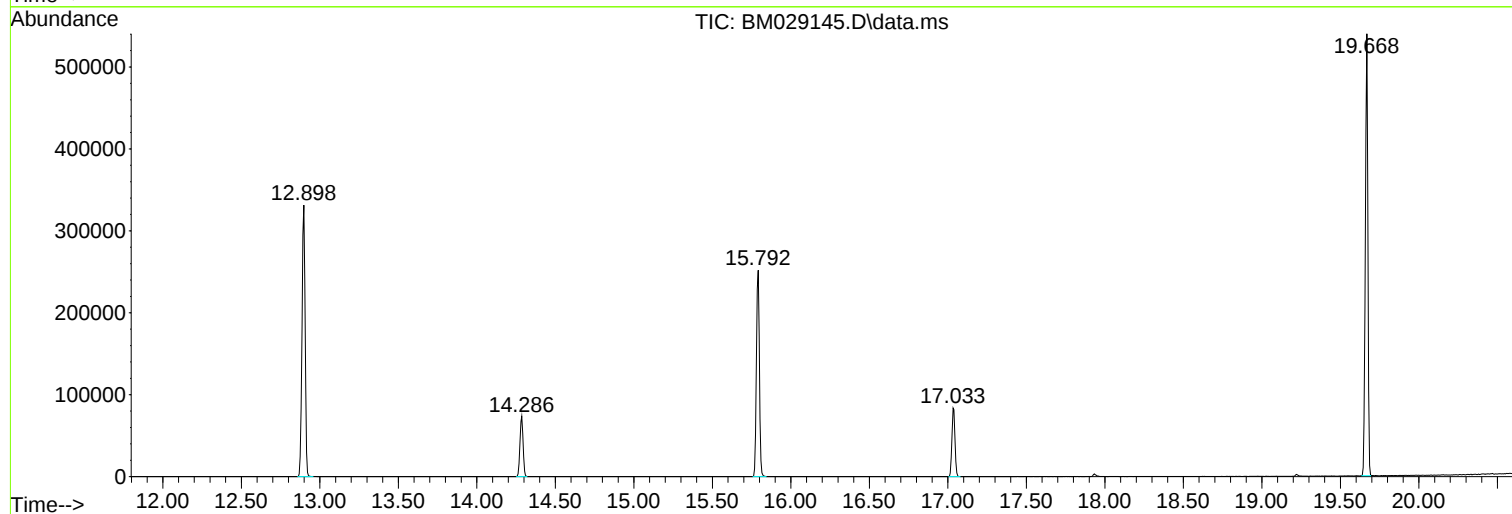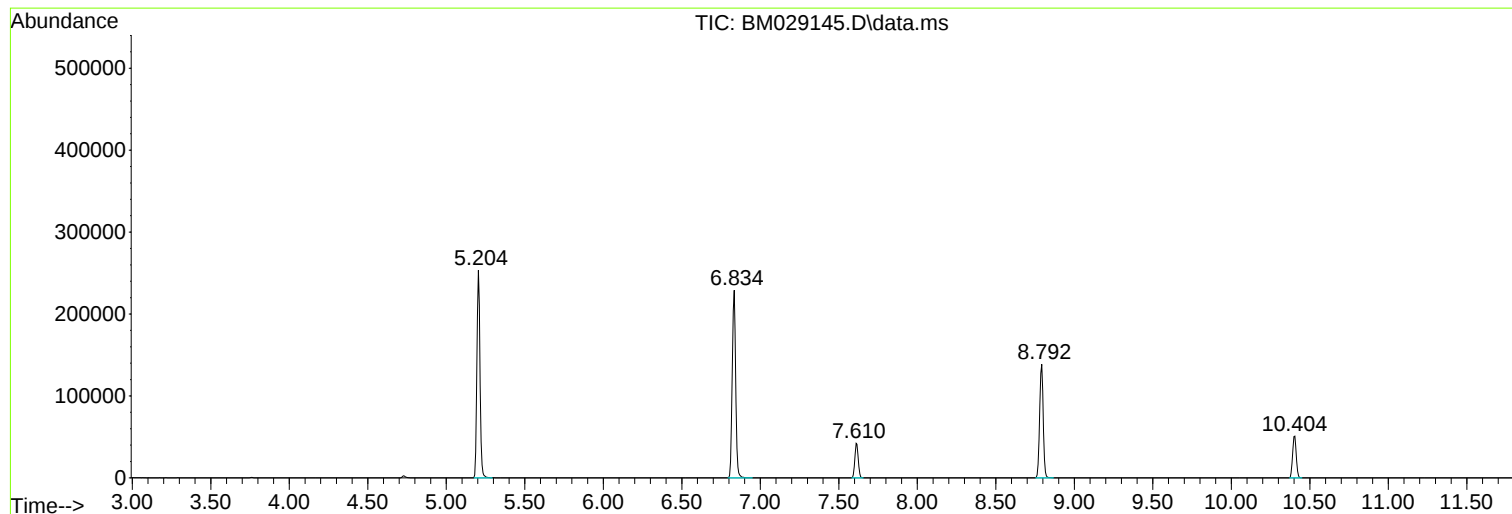

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031621\
Data File : BM029145.D
Acq On : 16 Mar 2021 12:14
Operator : CG/JU
Sample : PB135177BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135177BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031621\
Data File : BM029145.D
Acq On : 16 Mar 2021 12:14
Operator : CG/JU
Sample : PB135177BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135177BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------