

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031621\
 Data File : BM029150.D
 Acq On : 16 Mar 2021 16:00
 Operator : CG/JU
 Sample : PB135174BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135174BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029150.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.198	371	376	391	rBB	124800	186961	25.84%	6.543%
2	6.828	647	653	671	rBB	126314	195879	27.07%	6.855%
3	7.610	781	786	794	rBB	40564	61148	8.45%	2.140%
4	7.928	834	840	849	rBB	165908	249820	34.53%	8.743%
5	8.792	980	987	997	rBV	126943	202858	28.04%	7.100%
6	10.404	1255	1261	1270	rBB	52920	85006	11.75%	2.975%
7	12.898	1678	1685	1700	rBB	326331	449763	62.16%	15.741%
8	14.286	1915	1921	1928	rBB	76197	106357	14.70%	3.722%
9	15.786	2171	2176	2186	rBB	154739	213411	29.49%	7.469%
10	17.033	2383	2388	2396	rBB	90487	123691	17.09%	4.329%
11	19.668	2830	2836	2840	rBV	637680	723553	100.00%	25.322%
12	21.215	3094	3099	3106	rVB	112817	130111	17.98%	4.554%
13	23.350	3456	3462	3470	rBV2	71807	128796	17.80%	4.508%




Sum of corrected areas: 2857354

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031621\
Data File : BM029150.D
Acq On : 16 Mar 2021 16:00
Operator : CG/JU
Sample : PB135174BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

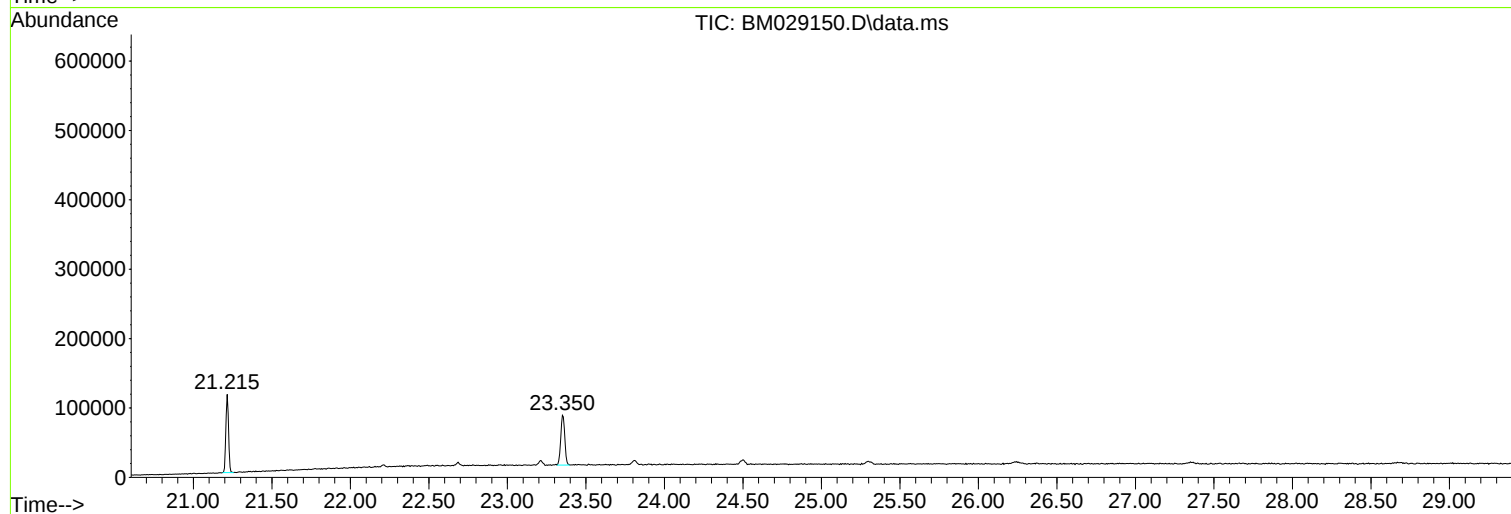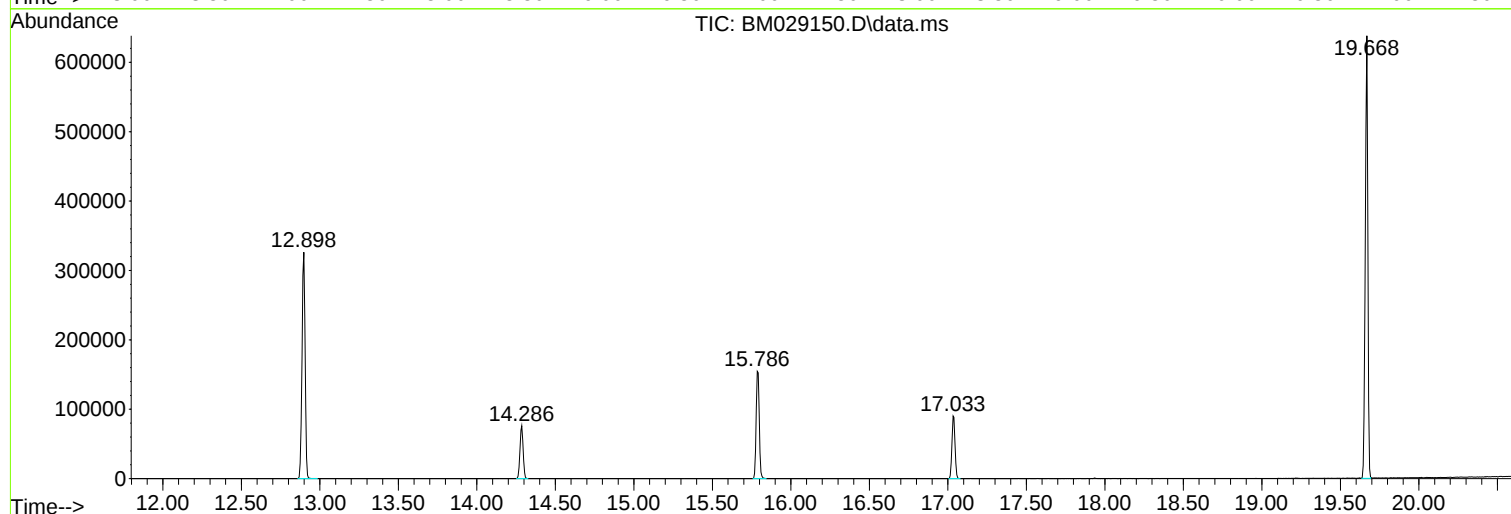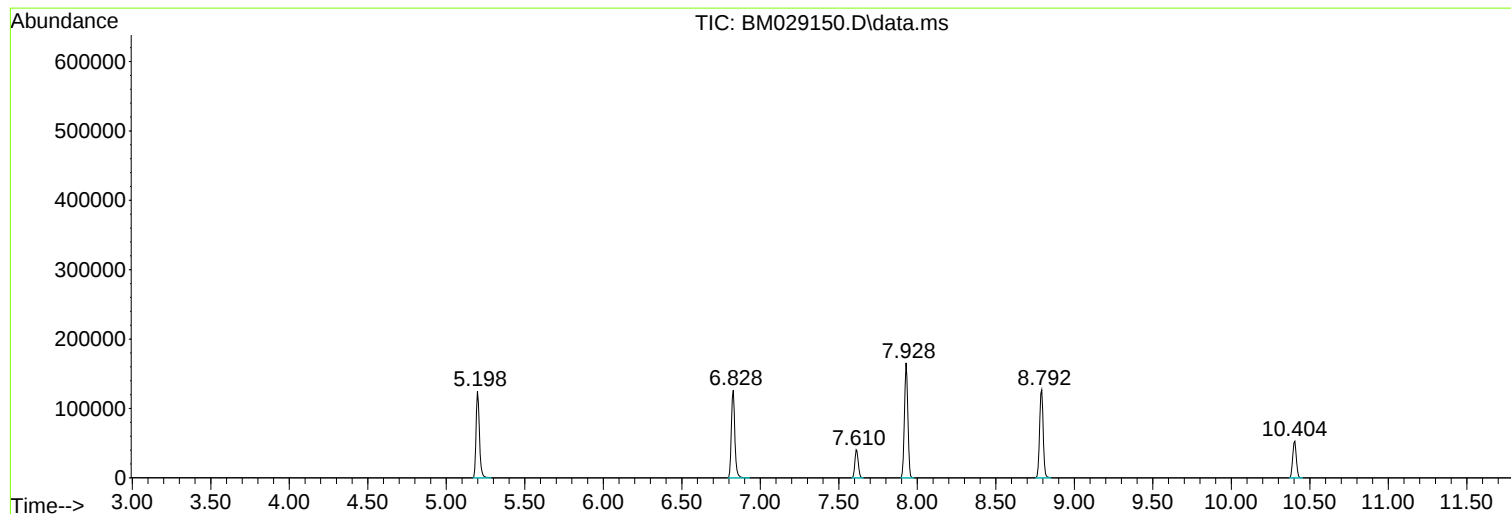

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031621\
Data File : BM029150.D
Acq On : 16 Mar 2021 16:00
Operator : CG/JU
Sample : PB135174BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031621\
Data File : BM029150.D
Acq On : 16 Mar 2021 16:00
Operator : CG/JU
Sample : PB135174BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135174BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM022321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------