
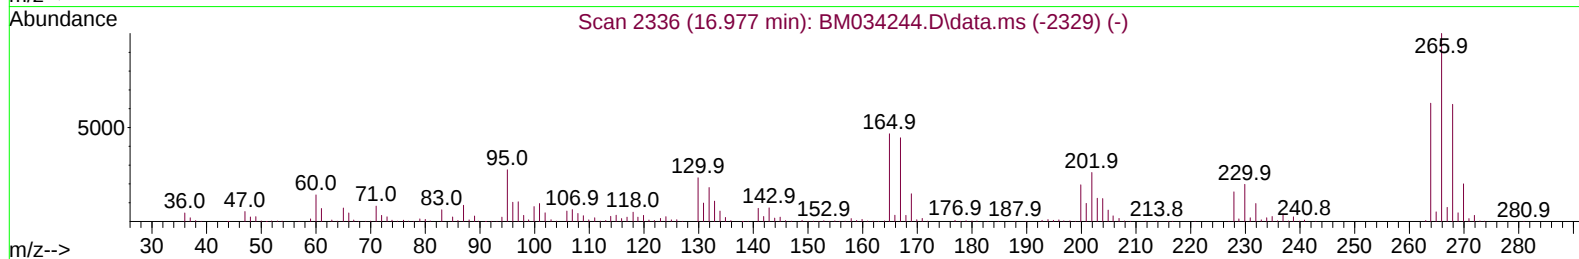
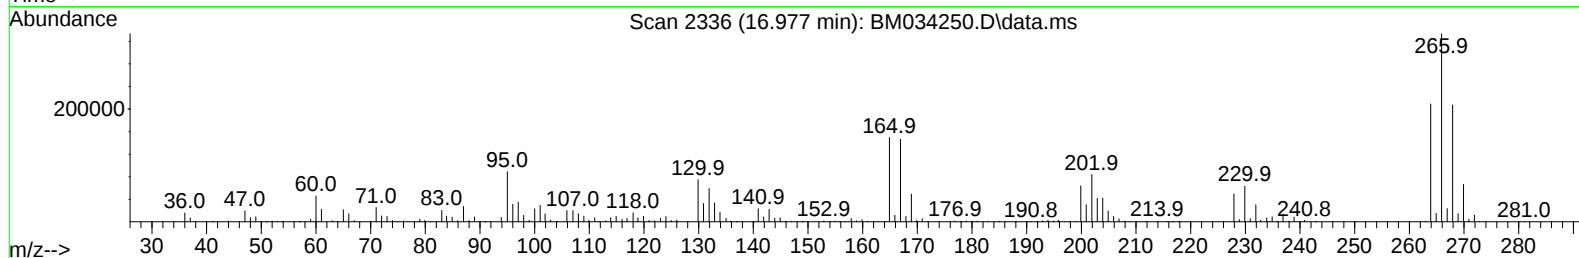


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034250.D
Acq On : 16 Mar 2022 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 12:39:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

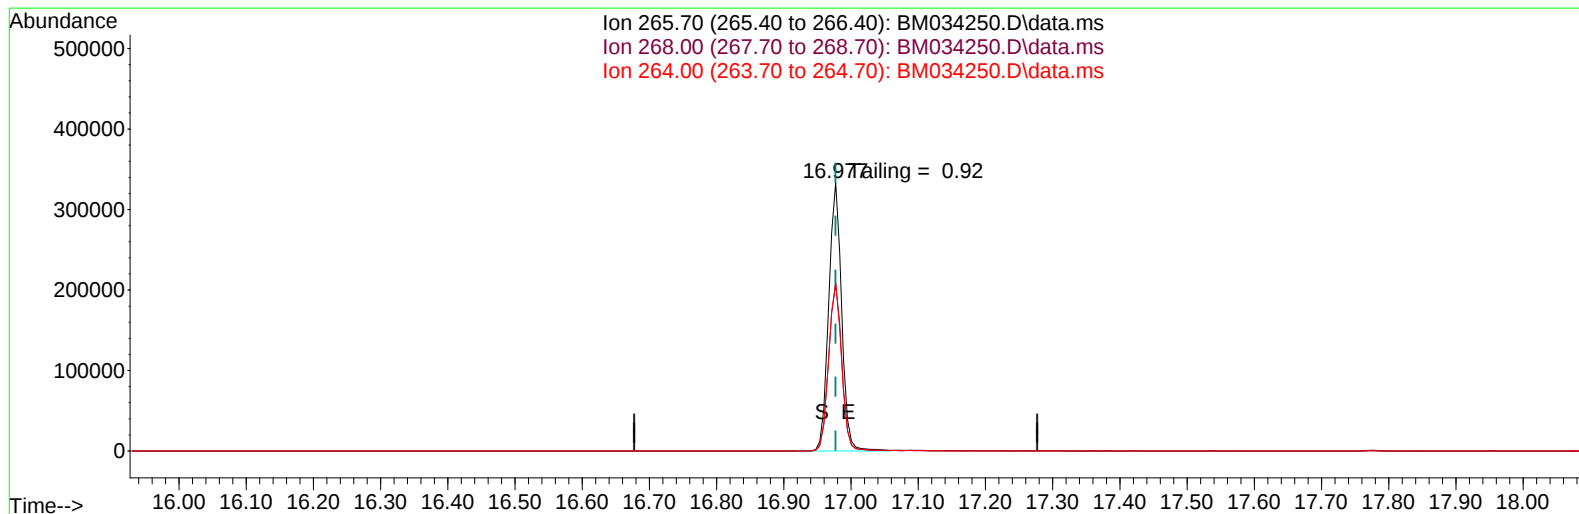

TIC: BM034250.D\data.ms

(70) Pentachlorophenol (C)




16.977min (-0.000) 632894.48 ng

response 446297

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.19
264.00	62.90	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034250.D
Acq On : 16 Mar 2022 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 16 12:39:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

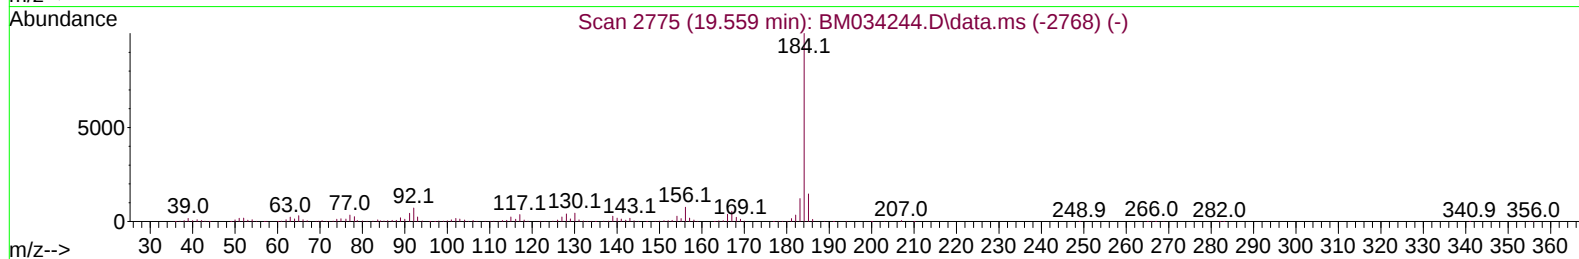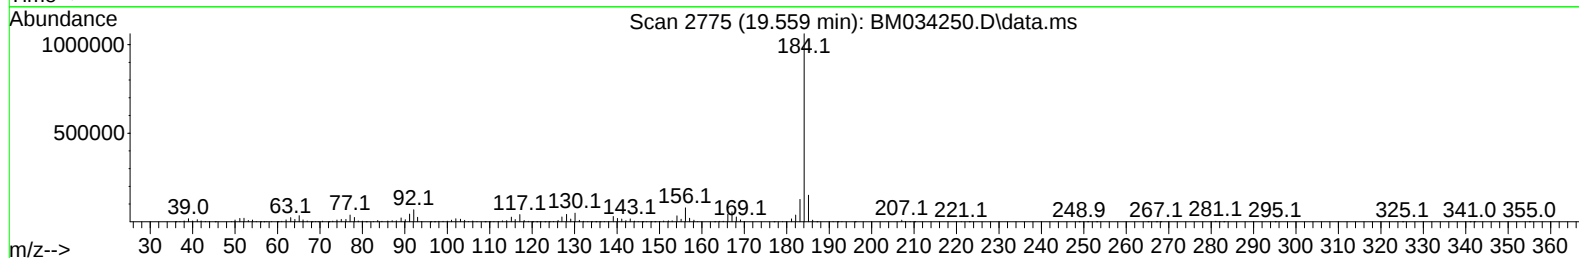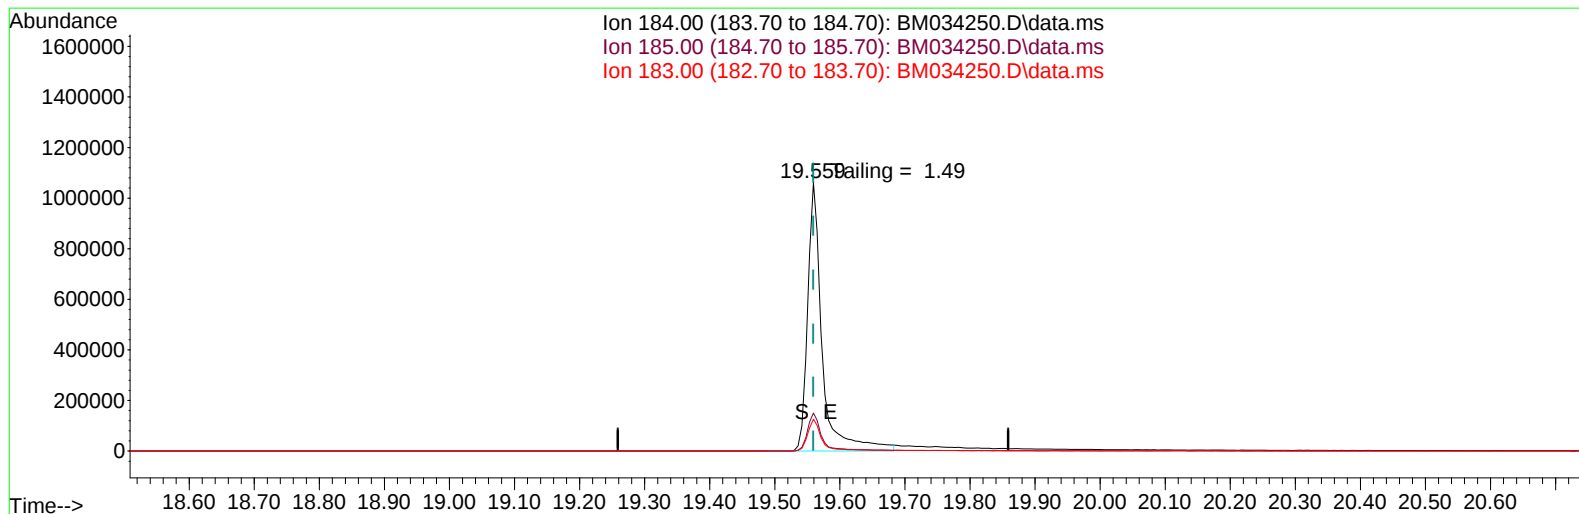

TIC: BM034250.D\data.ms

(77) Benzidine**19.559min (+ 0.000) 28686.25 ng****response 1723552**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.14
183.00	12.20	11.90
0.00	0.00	0.00