

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
 Data File : BM034252.D
 Acq On : 16 Mar 2022 10:38
 Operator : CG/JU
 Sample : PB143161BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143161BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.502	378	385	397	rBV	3783193	5380626	62.09%	12.140%
2	7.107	650	658	675	rBV	3421675	5462858	63.04%	12.326%
3	7.949	794	801	814	rVB	628748	999561	11.53%	2.255%
4	9.107	990	998	1020	rBV	2050475	3534697	40.79%	7.975%
5	10.760	1268	1279	1288	rBV	752728	1302644	15.03%	2.939%
6	13.219	1689	1697	1708	rBV	5189244	7780869	89.79%	17.556%
7	14.583	1923	1929	1942	rBV	1096187	1631700	18.83%	3.682%
8	16.066	2174	2181	2196	rBV	3650392	5325414	61.46%	12.016%
9	17.324	2388	2395	2409	rBV	1103921	1672003	19.29%	3.773%
10	19.942	2834	2840	2859	rBV	7083572	8665494	100.00%	19.552%
11	21.495	3099	3104	3111	rBV	900898	1317771	15.21%	2.973%
12	23.906	3508	3514	3530	rVB	551858	1246899	14.39%	2.813%




Sum of corrected areas: 44320536

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034252.D
Acq On : 16 Mar 2022 10:38
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

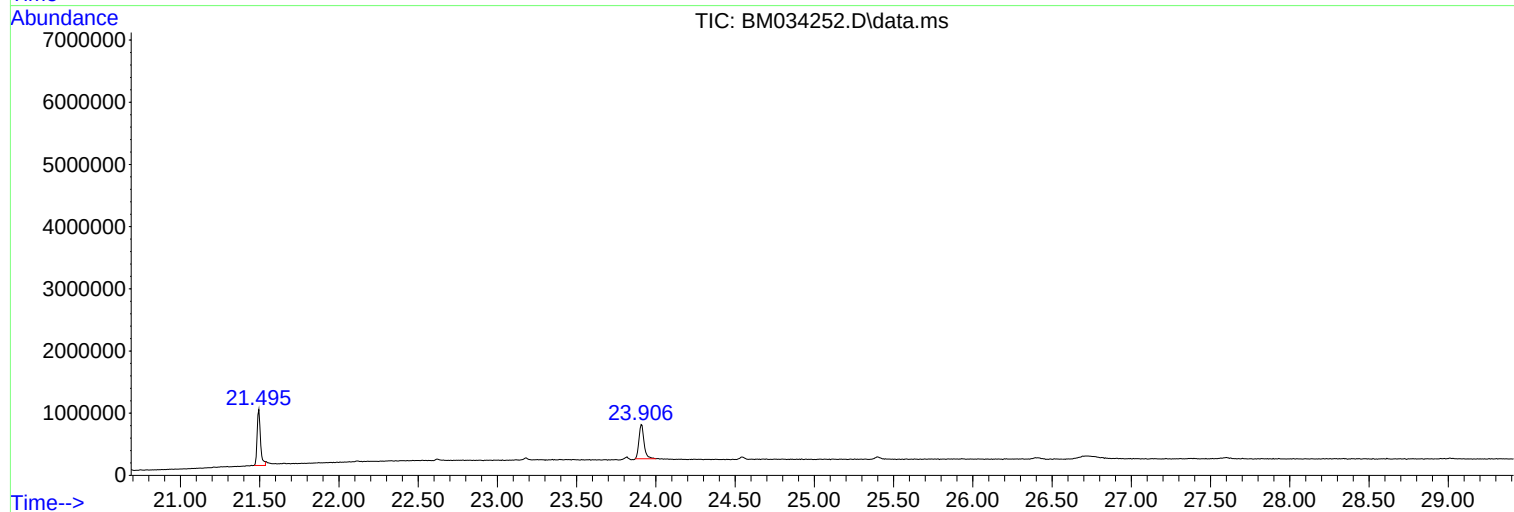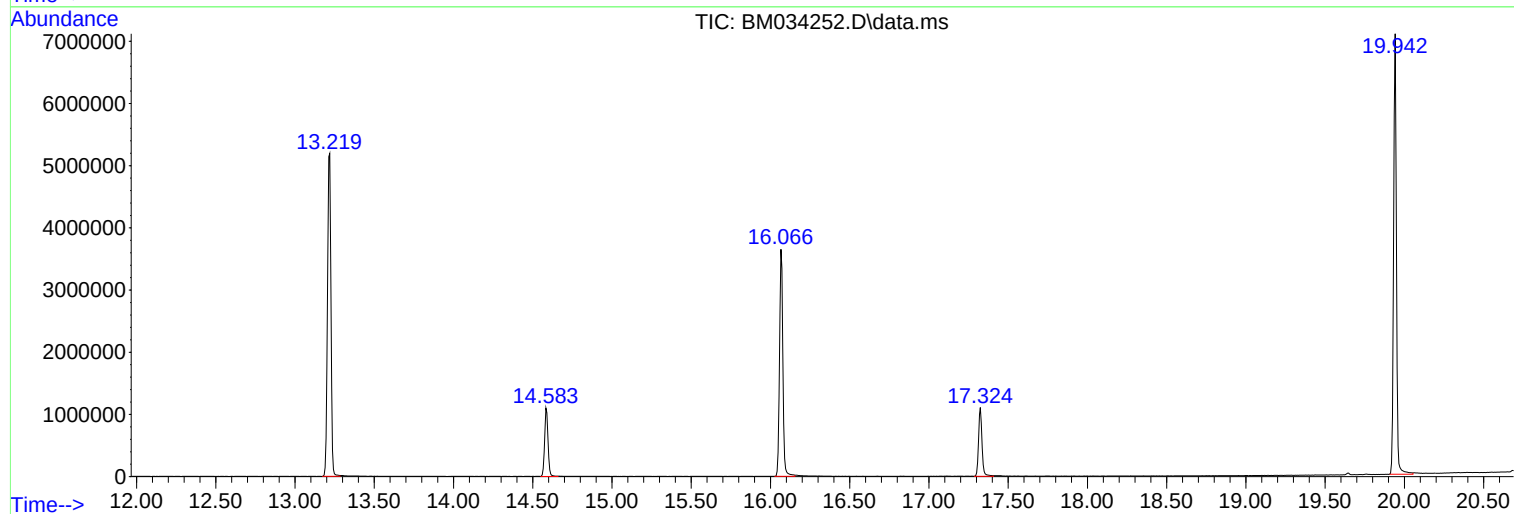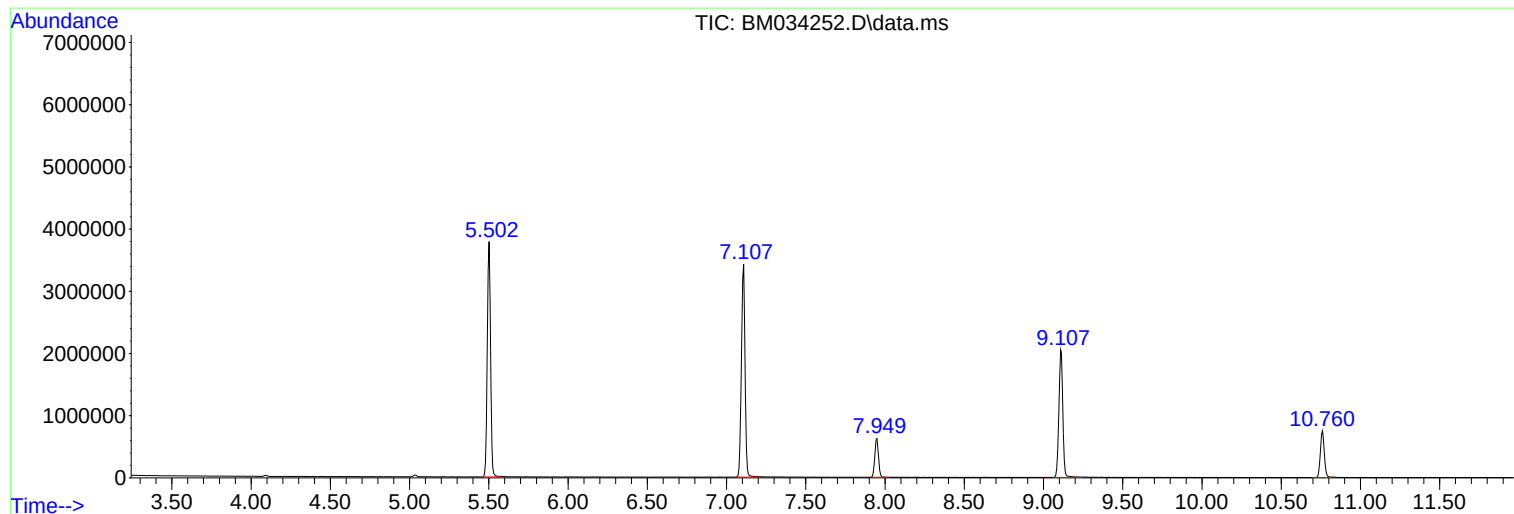

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034252.D
Acq On : 16 Mar 2022 10:38
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034252.D
Acq On : 16 Mar 2022 10:38
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------