

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
 Data File : BM034257.D
 Acq On : 16 Mar 2022 13:43
 Operator : CG/JU
 Sample : PB143171BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143171BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.501	378	385	398	rBV	3300787	4632635	69.53%	13.027%
2	7.107	650	658	667	rBV	2860288	4530476	68.00%	12.739%
3	7.948	795	801	809	rBV	562669	879019	13.19%	2.472%
4	9.107	990	998	1010	rBV	1738070	2943435	44.18%	8.277%
5	10.760	1271	1279	1296	rBV	631861	1098515	16.49%	3.089%
6	13.219	1689	1697	1721	rBV	4111519	6116787	91.81%	17.200%
7	14.583	1923	1929	1943	rBV	807020	1237531	18.57%	3.480%
8	16.065	2174	2181	2203	rBV	2642296	3867469	58.05%	10.875%
9	17.324	2389	2395	2411	rBV	809538	1212051	18.19%	3.408%
10	19.942	2834	2840	2857	rBV	5151374	6662491	100.00%	18.734%
11	21.494	3099	3104	3121	rBV	747306	1233831	18.52%	3.469%
12	23.906	3508	3514	3524	rBV2	503143	1148759	17.24%	3.230%


Sum of corrected areas: 35562999

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034257.D
Acq On : 16 Mar 2022 13:43
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

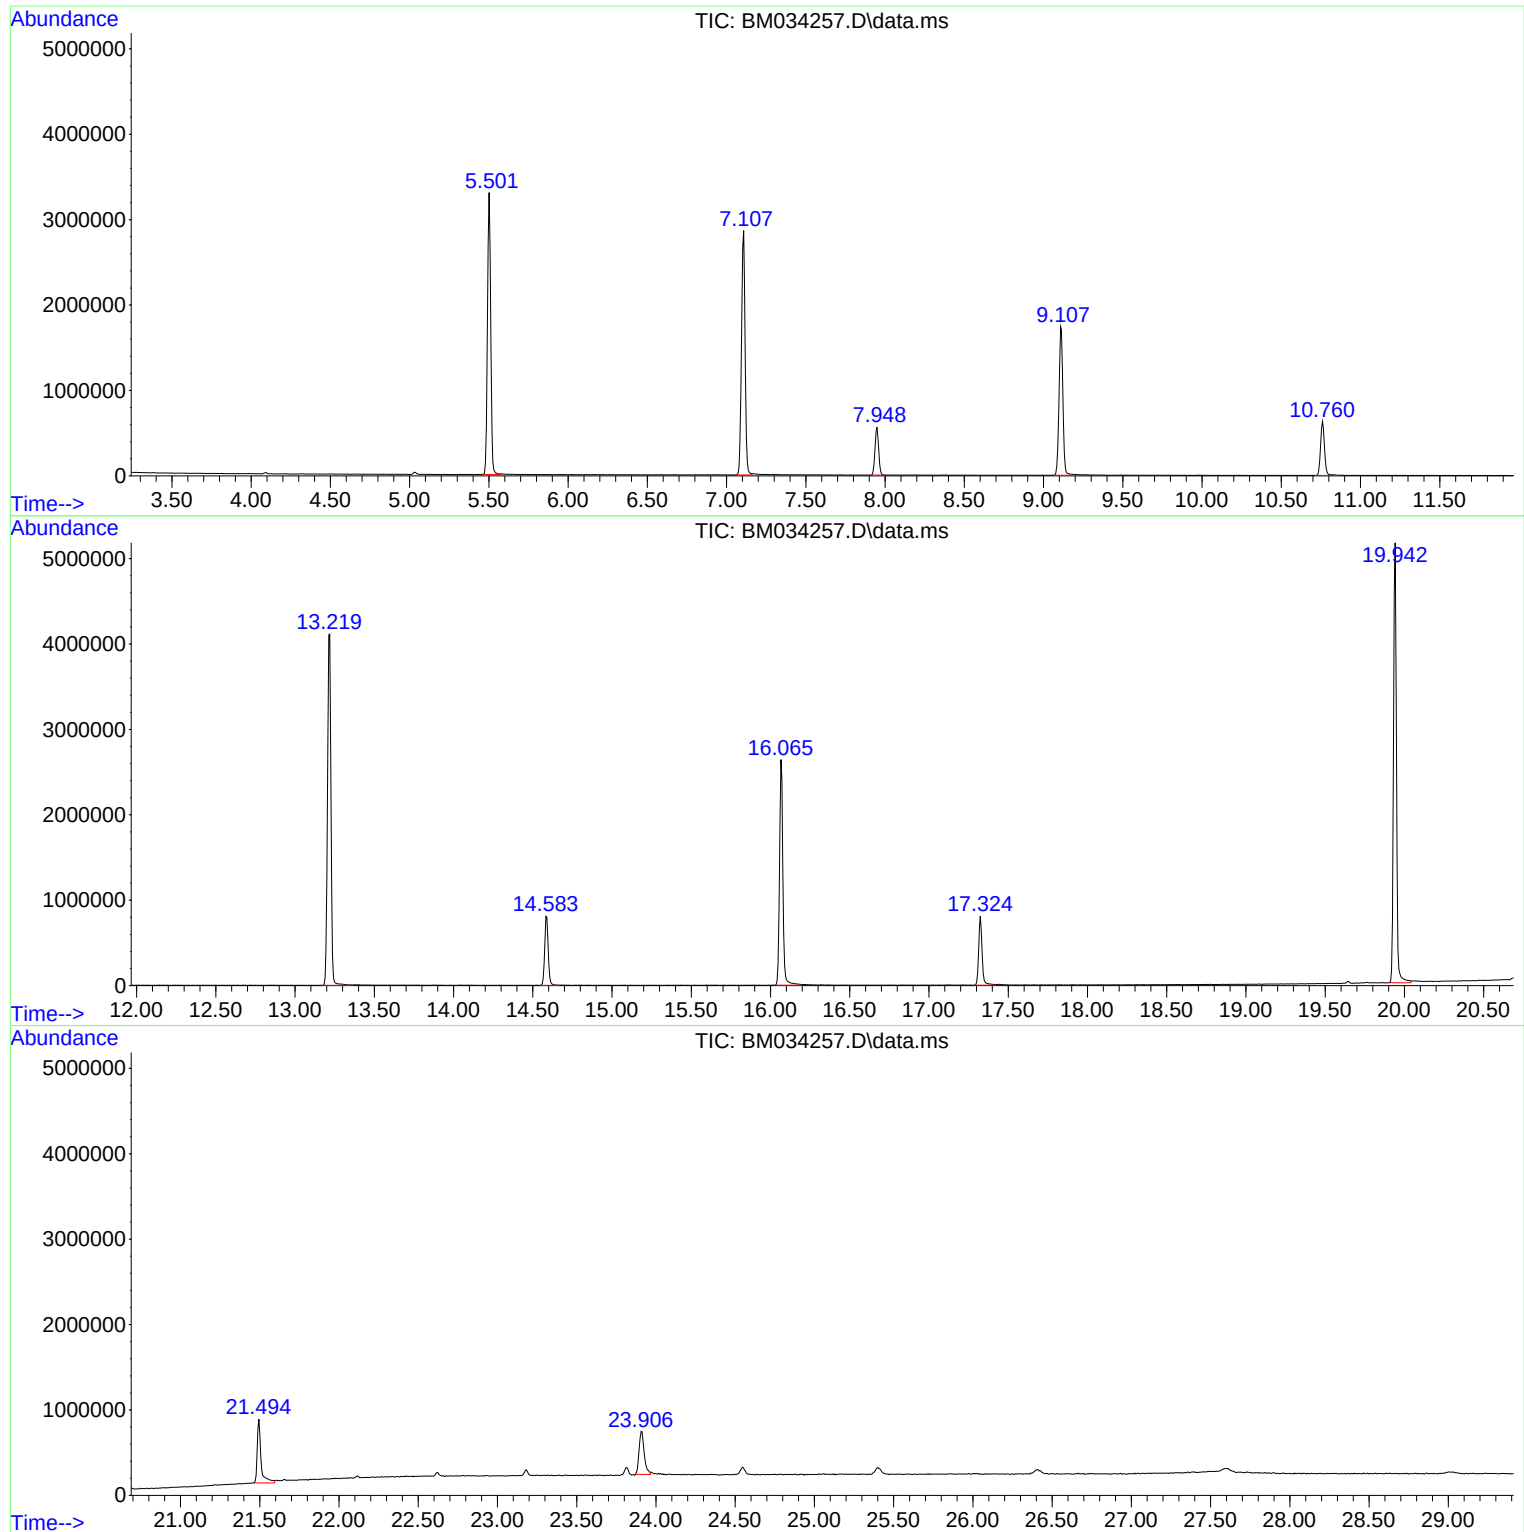

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034257.D
Acq On : 16 Mar 2022 13:43
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034257.D
Acq On : 16 Mar 2022 13:43
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------