

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
 Data File : BM034264.D
 Acq On : 16 Mar 2022 19:13
 Operator : CG/JU
 Sample : PB143171BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143171BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.501	378	385	395	rBV	2744505	4006464	36.81%	9.259%
2	7.107	650	658	673	rBV	2637350	4253582	39.08%	9.831%
3	7.948	793	801	808	rBV	516284	817331	7.51%	1.889%
4	9.107	991	998	1013	rBV	1587540	2684144	24.66%	6.203%
5	10.760	1271	1279	1289	rBV	659521	1129867	10.38%	2.611%
6	13.219	1689	1697	1709	rBV	4290138	6403493	58.84%	14.799%
7	14.583	1923	1929	1942	rBV	1030776	1607424	14.77%	3.715%
8	16.065	2175	2181	2199	rBV	3531421	5263134	48.36%	12.164%
9	17.324	2388	2395	2411	rBV	1305440	1946469	17.88%	4.499%
10	19.942	2834	2840	2861	rBV	8671626	10883608	100.00%	25.153%
11	21.494	3099	3104	3119	rBV	1501811	2193127	20.15%	5.069%
12	23.912	3508	3515	3530	rBV2	935372	2080232	19.11%	4.808%




Sum of corrected areas: 43268875

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034264.D
Acq On : 16 Mar 2022 19:13
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

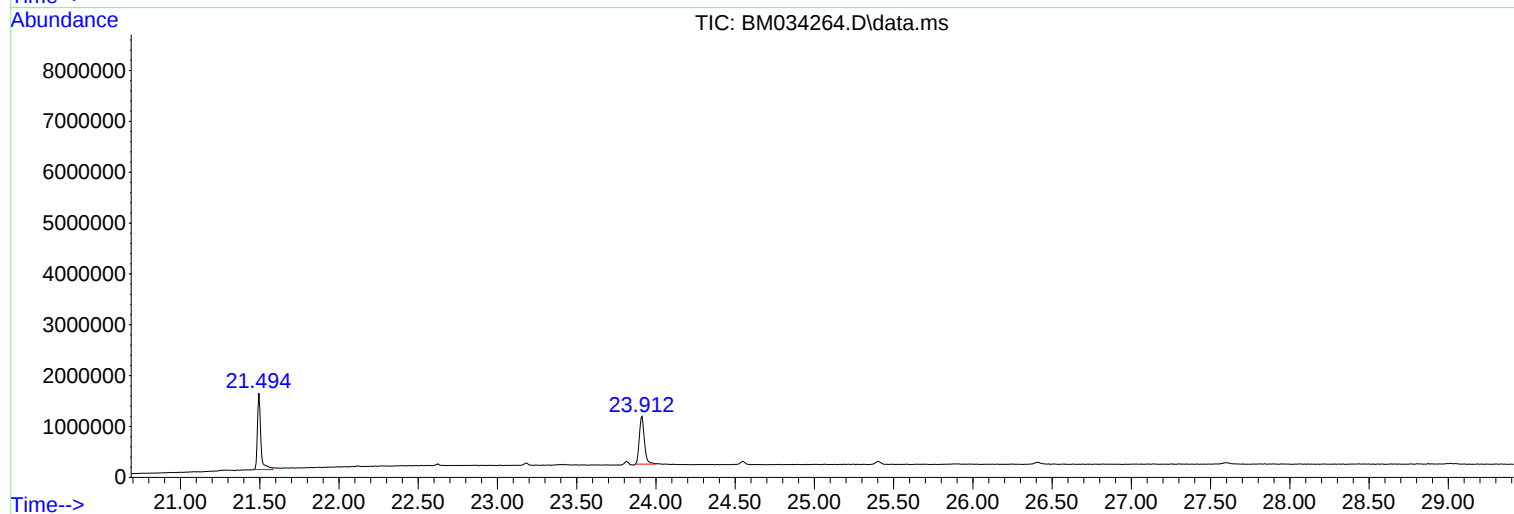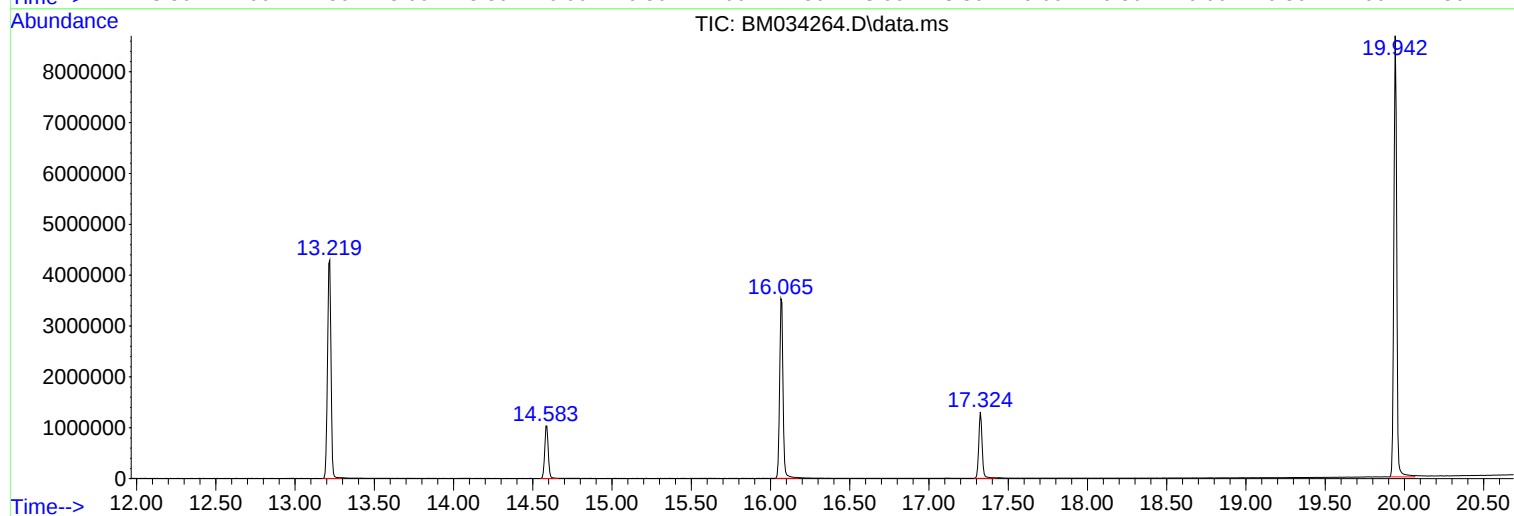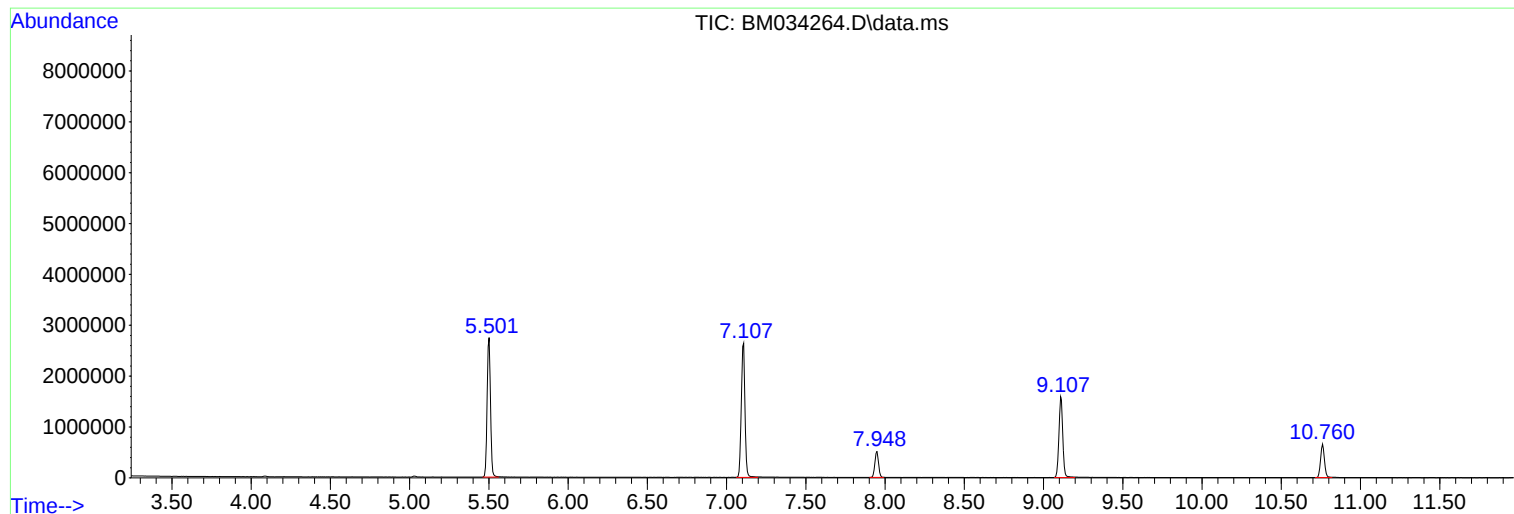

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034264.D
Acq On : 16 Mar 2022 19:13
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034264.D
Acq On : 16 Mar 2022 19:13
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------