


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
 Data File : BM034250.D
 Acq On : 16 Mar 2022 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 16 02:38:26 2022

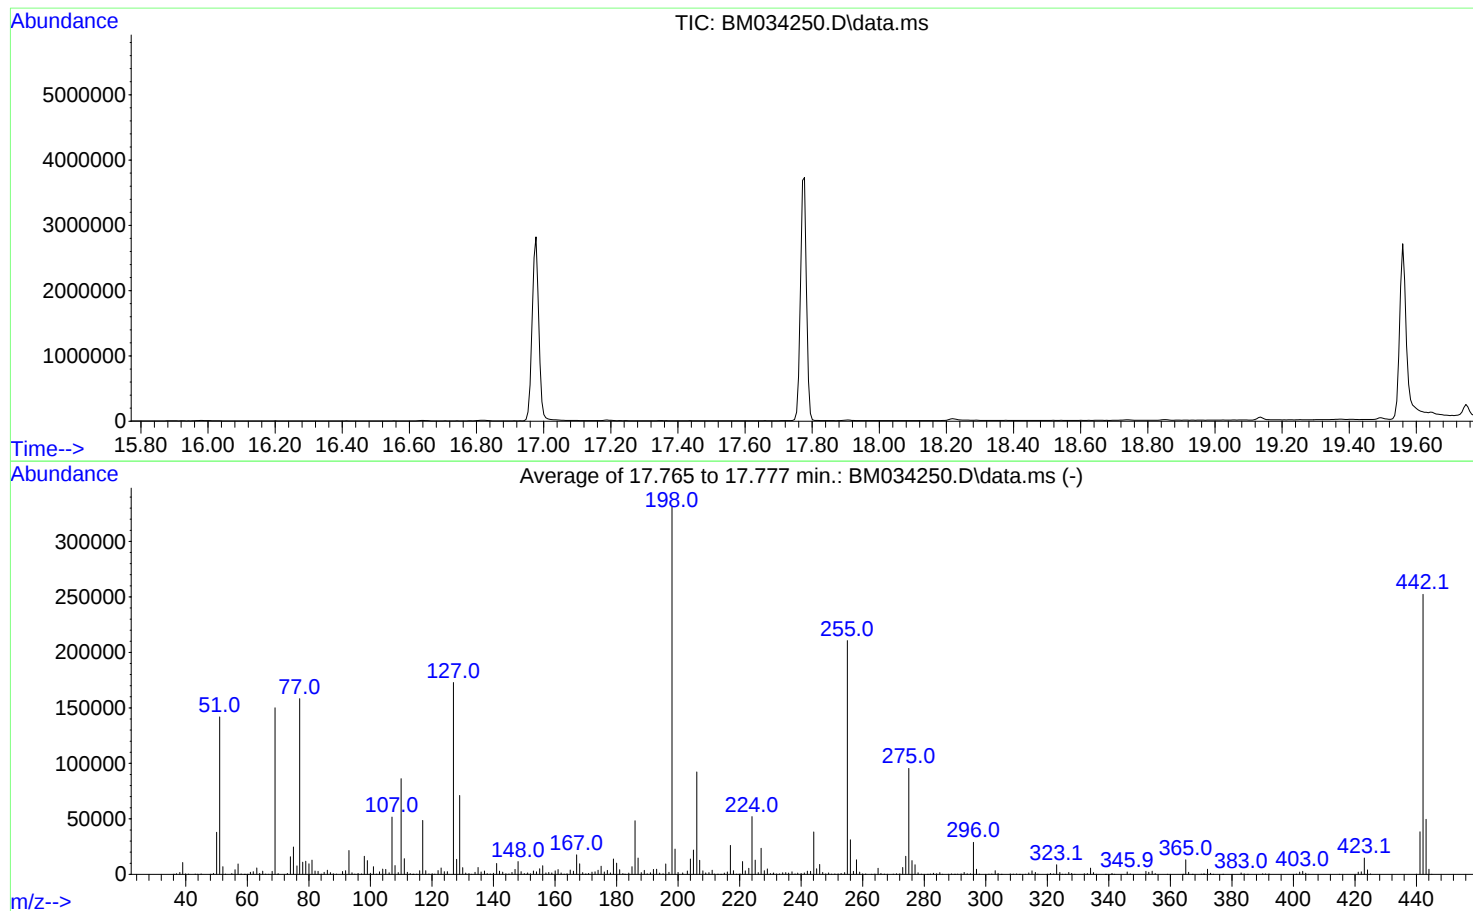




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	141861	PASS
68	69	0.00	2	1.8	2744	PASS
69	198	0.00	100	45.3	150051	PASS
70	69	0.00	2	0.4	592	PASS
127	198	10	80	52.1	172816	PASS
197	198	0.00	2	0.6	1877	PASS
198	198	100	100	100.0	331456	PASS
199	198	5	9	6.9	22746	PASS
275	198	10	60	28.8	95477	PASS
365	198	1	100	4.0	13108	PASS
441	198	0.01	100	11.6	38381	PASS
442	442	50	100	100.0	252339	PASS
443	442	15	24	19.7	49651	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
 Data File : BM034250.D
 Acq On : 16 Mar 2022 09:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 16 12:39:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 16 02:38:26 2022
 Response via : Initial Calibration

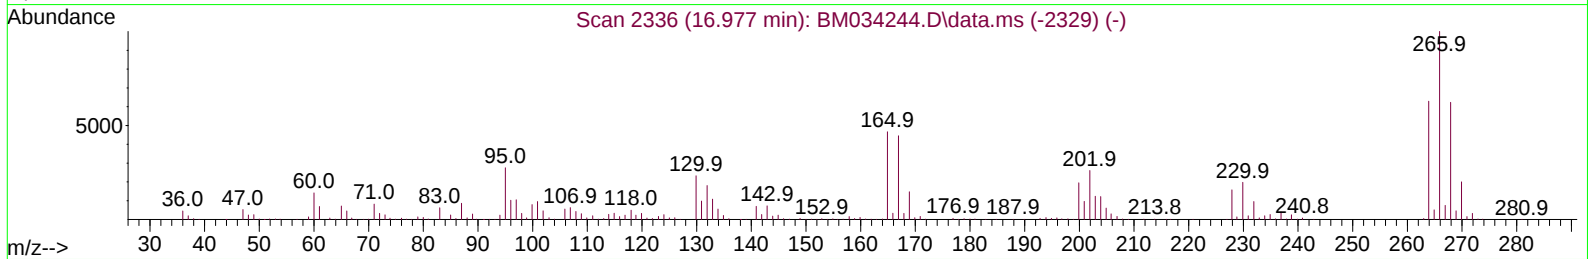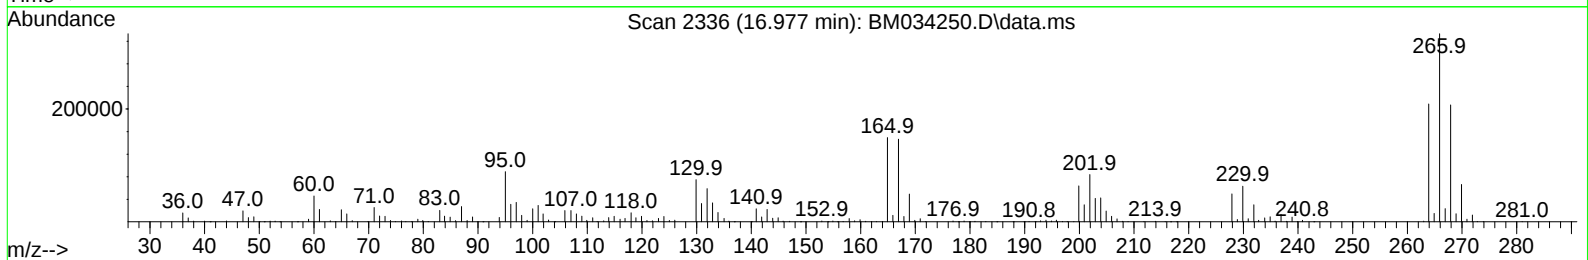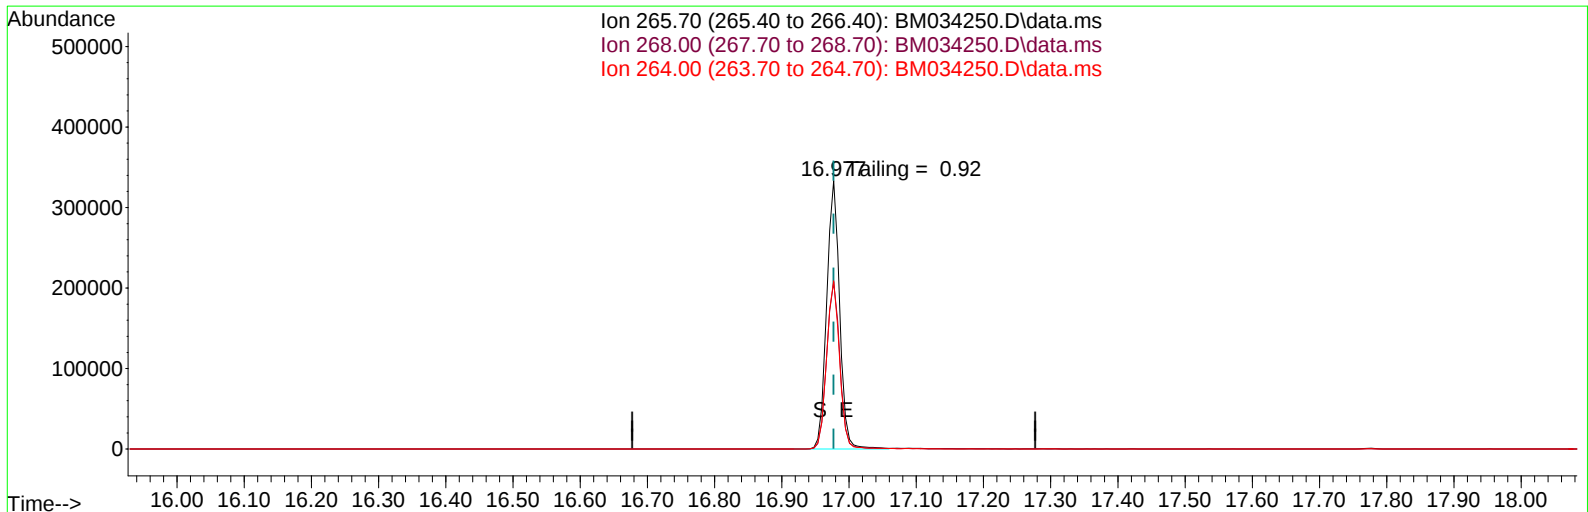

TIC: BM034250.D\data.ms

(70) Pentachlorophenol (C)

16.977min (-0.000) 632894.48 ng


response 446297

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.19
264.00	62.90	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031622\
Data File : BM034250.D
Acq On : 16 Mar 2022 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 16 12:39:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

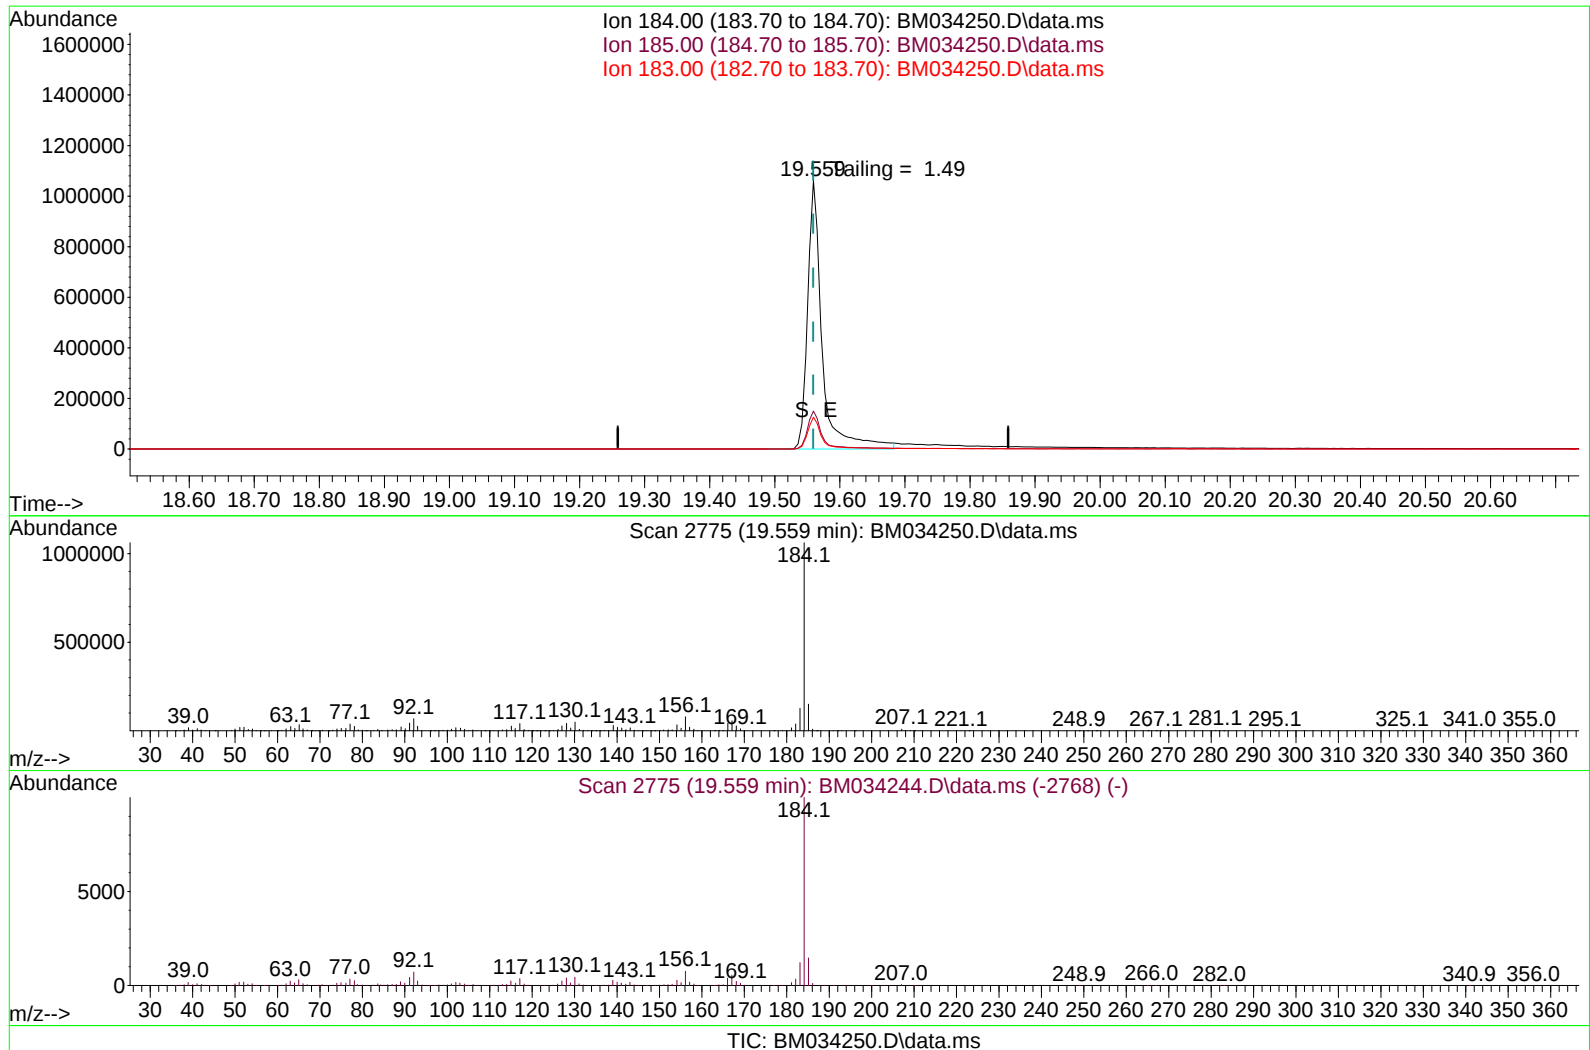

(77) Benzidine

19.559min (+ 0.000) 28686.25 ng

response 1723552

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.14
183.00	12.20	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/16/2022	BNA_M	<u>BM034250.D</u>
Compound Name	Response	Retention Time
DDT	1316652	20.8
DDD	6510	20.35
DDE	1022	19.85
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7532	1324184	0.57

Instrument :
BNA_M
ClientSampleId :
DFTPP