

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031824\
 Data File : BM044656.D
 Acq On : 18 Mar 2024 13:12
 Operator : MA/JU
 Sample : P1747-03RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MW-01RE

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM044656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.863	297	302	312	rVB	393797	528365	5.04%	1.149%
2	5.304	370	377	387	rBV	1346348	1962399	18.71%	4.269%
3	6.869	636	643	652	rBV	704685	1139997	10.87%	2.480%
4	7.698	777	784	790	rBV	771051	1229186	11.72%	2.674%
5	7.757	790	794	802	rVB	73124	115605	1.10%	0.251%
6	8.857	974	981	996	rBV	2668993	4400988	41.96%	9.573%
7	10.475	1249	1256	1264	rBV	903598	1589388	15.15%	3.457%
8	11.739	1462	1471	1484	rBV	91859	184962	1.76%	0.402%
9	12.957	1671	1678	1691	rBV	5760532	8891179	84.77%	19.340%
10	14.339	1907	1913	1922	rBV	1259767	1868843	17.82%	4.065%
11	14.568	1946	1952	1962	rBV	81649	123107	1.17%	0.268%
12	15.098	2037	2042	2048	rBV	130889	191169	1.82%	0.416%
13	15.562	2114	2121	2133	rBV	402456	602240	5.74%	1.310%
14	15.839	2161	2168	2178	rBV	3020430	4167688	39.74%	9.065%
15	17.098	2375	2382	2392	rBV	1443795	2060935	19.65%	4.483%
16	18.003	2531	2536	2545	rBV	174864	260016	2.48%	0.566%
17	19.292	2751	2755	2764	rBV	114434	172857	1.65%	0.376%
18	19.744	2825	2832	2846	rBV	8103101	10488582	100.00%	22.815%
19	21.027	3046	3050	3058	rBV2	138334	209423	2.00%	0.456%
20	21.297	3090	3096	3103	rBV	1783735	2312133	22.04%	5.029%
21	21.909	3197	3200	3209	rBV2	75121	116374	1.11%	0.253%
22	22.080	3224	3229	3237	rBV	567731	760853	7.25%	1.655%
23	23.544	3471	3478	3490	rVB	1355355	2596966	24.76%	5.649%




Sum of corrected areas: 45973255

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031824\
Data File : BM044656.D
Acq On : 18 Mar 2024 13:12
Operator : MA/JU
Sample : P1747-03RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

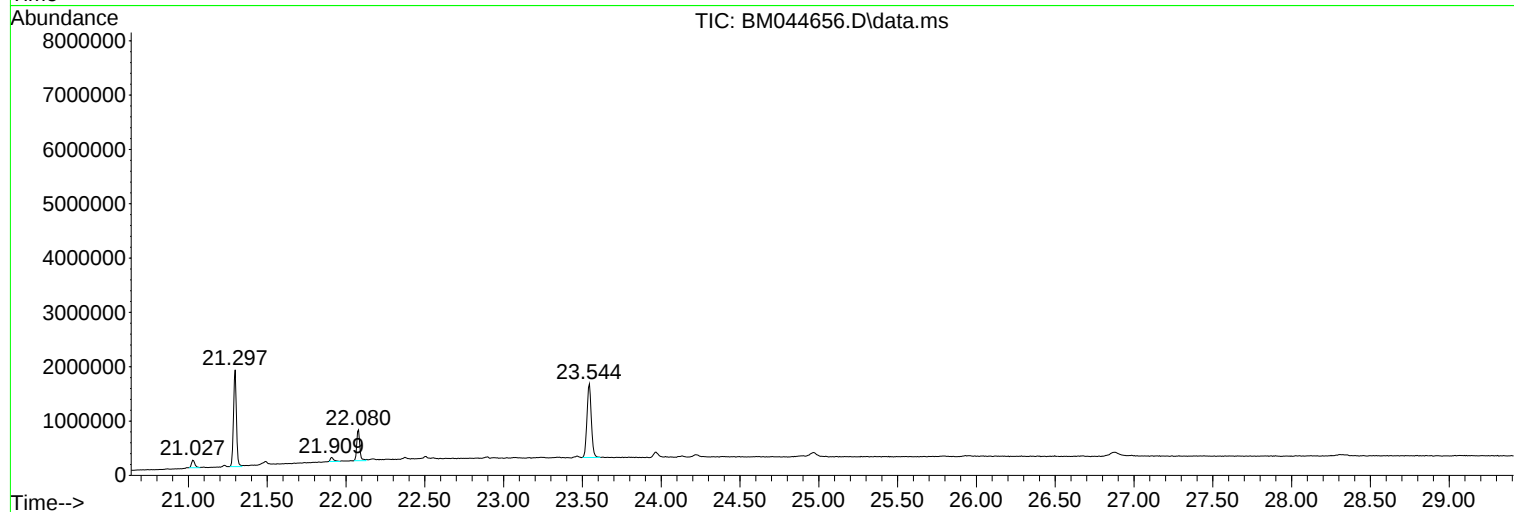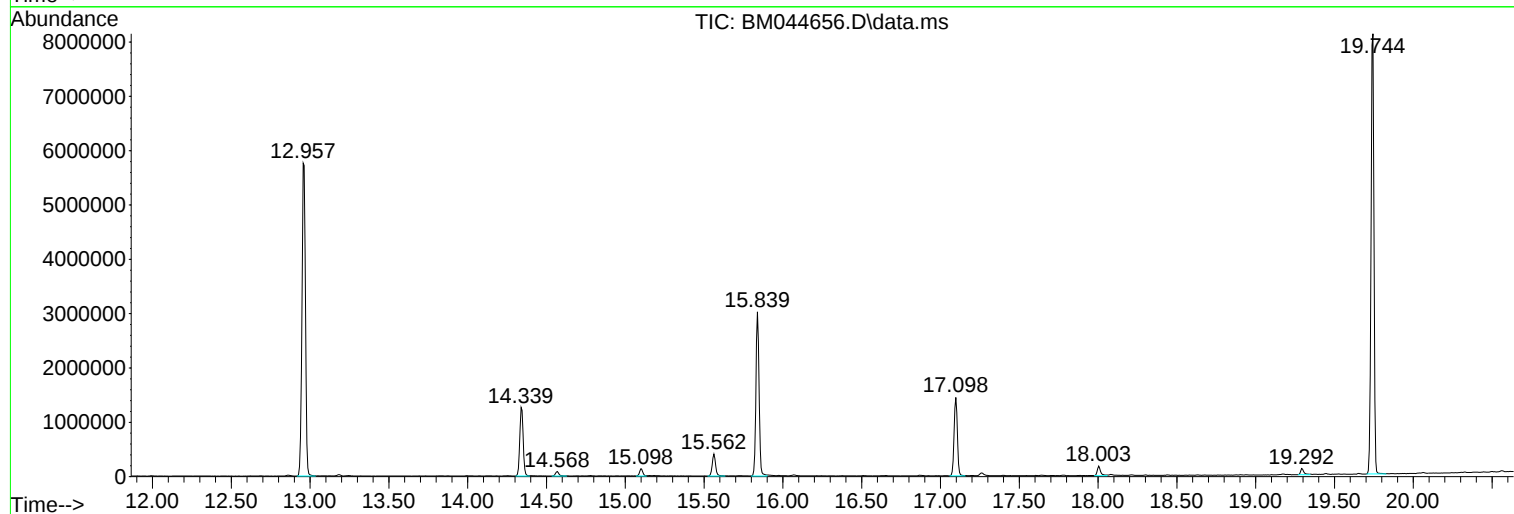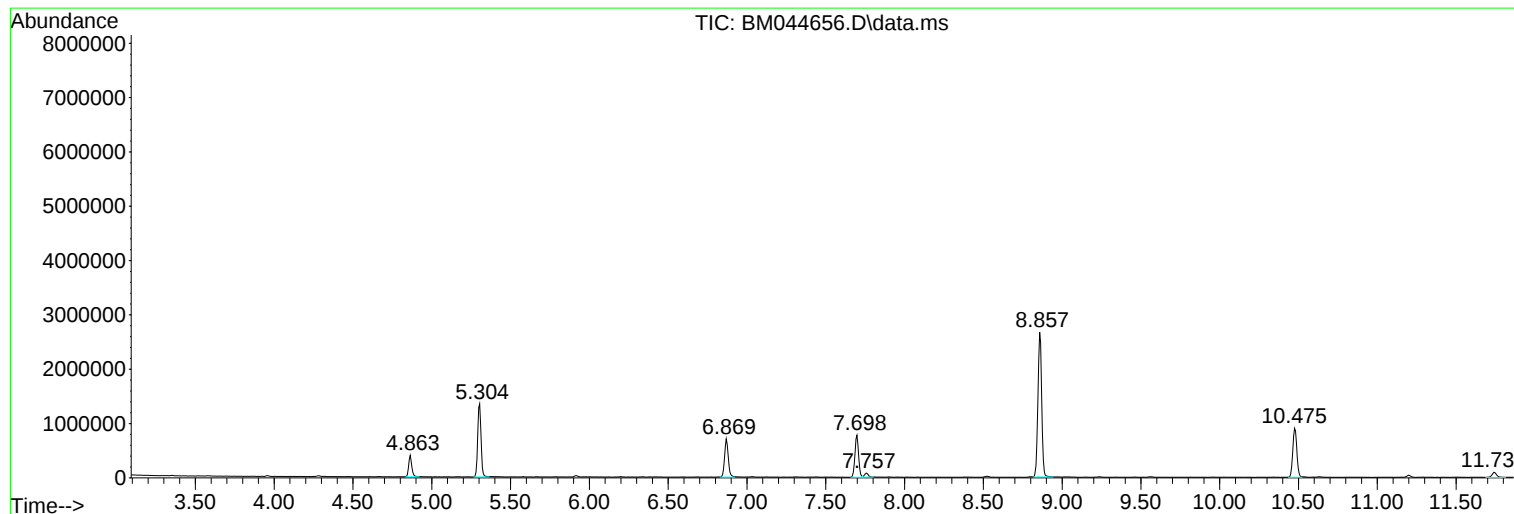

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031824\
Data File : BM044656.D
Acq On : 18 Mar 2024 13:12
Operator : MA/JU
Sample : P1747-03RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031824\
Data File : BM044656.D
Acq On : 18 Mar 2024 13:12
Operator : MA/JU
Sample : P1747-03RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MW-01RE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------