


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031824\
Data File : BM044653.D
Acq On : 18 Mar 2024 11:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 14 02:28:24 2024

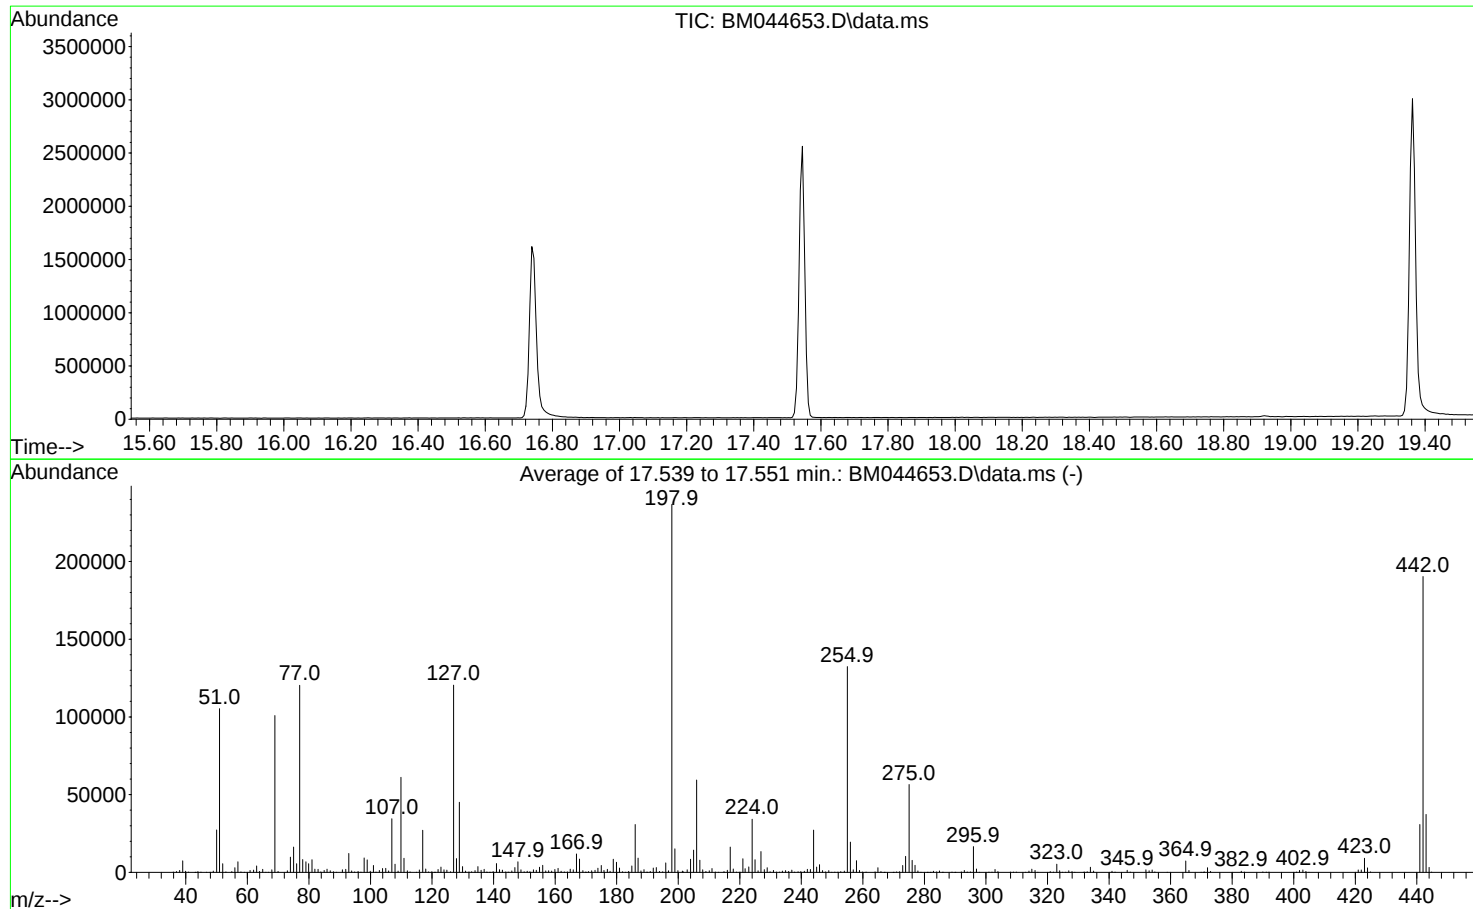




AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.5	105319	PASS
68	69	0.00	2	1.6	1622	PASS
69	198	0.00	100	42.6	100848	PASS
70	69	0.00	2	0.6	654	PASS
127	198	10	80	50.9	120485	PASS
197	198	0.00	2	0.4	1037	PASS
198	198	100	100	100.0	236672	PASS
199	198	5	9	6.4	15125	PASS
275	198	10	60	23.9	56501	PASS
365	198	1	100	3.1	7296	PASS
441	198	0.01	100	13.0	30816	PASS
442	442	50	100	100.0	190379	PASS
443	442	15	24	19.6	37288	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031824\
Data File : BM044653.D
Acq On : 18 Mar 2024 11:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 19 00:47:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration

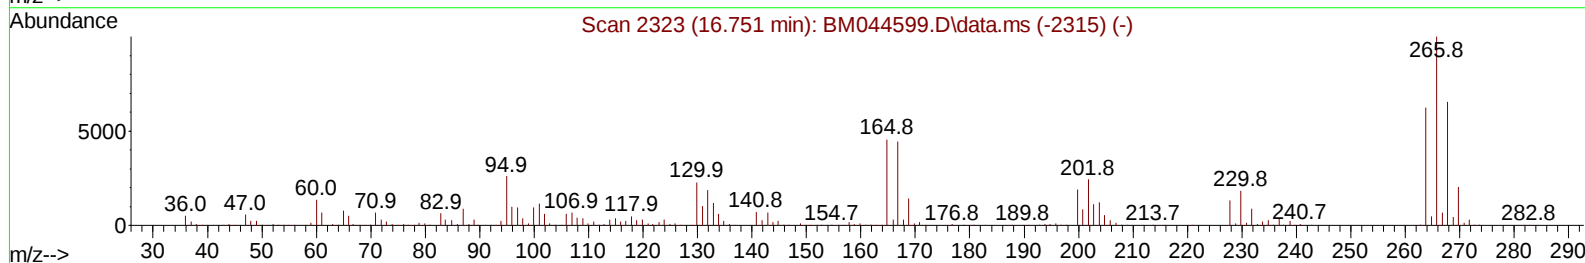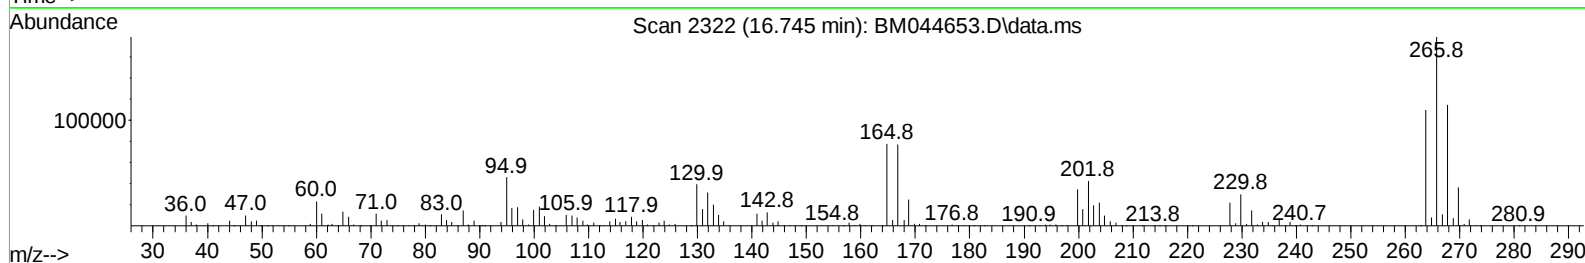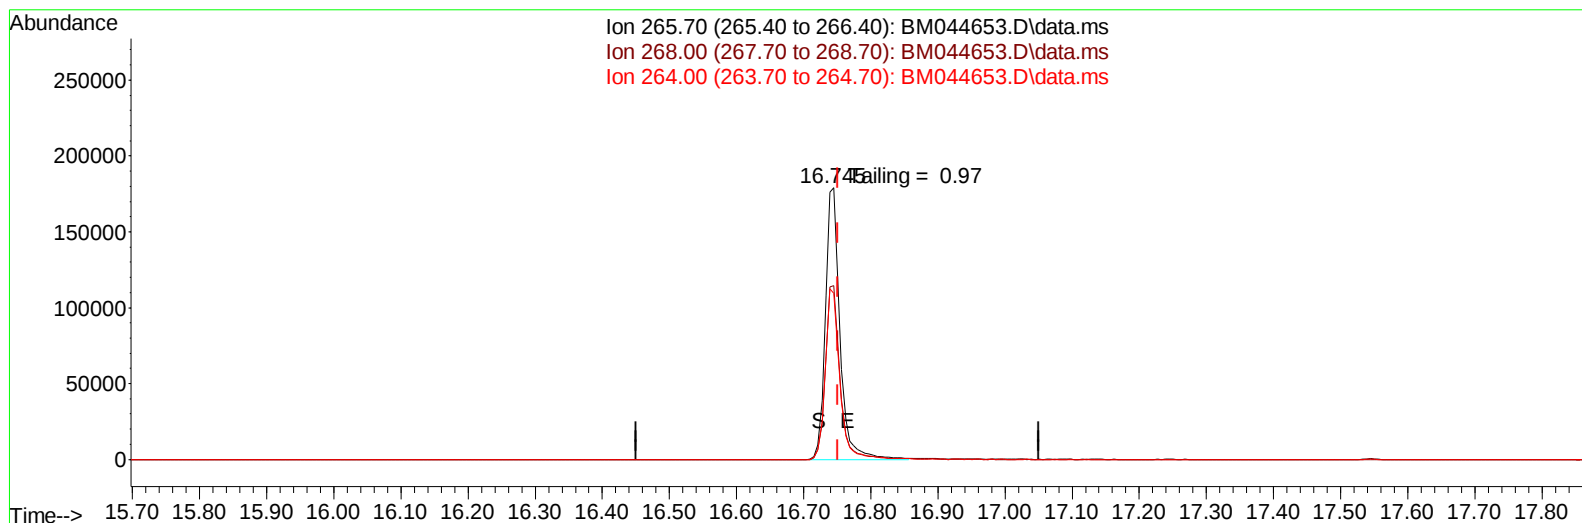

TIC: BM044653.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.006) 0.00 ng




response 273803

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	64.00
264.00	62.30	61.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031824\
Data File : BM044653.D
Acq On : 18 Mar 2024 11:14
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 19 00:47:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 14 02:28:24 2024
Response via : Initial Calibration

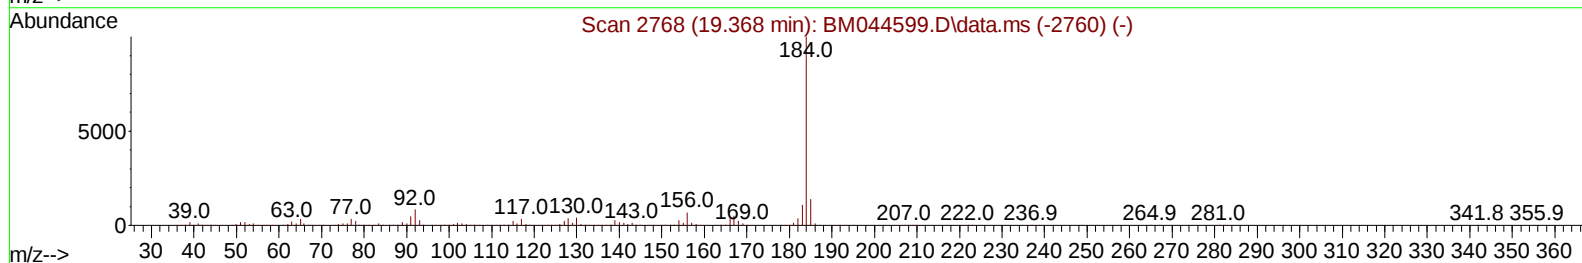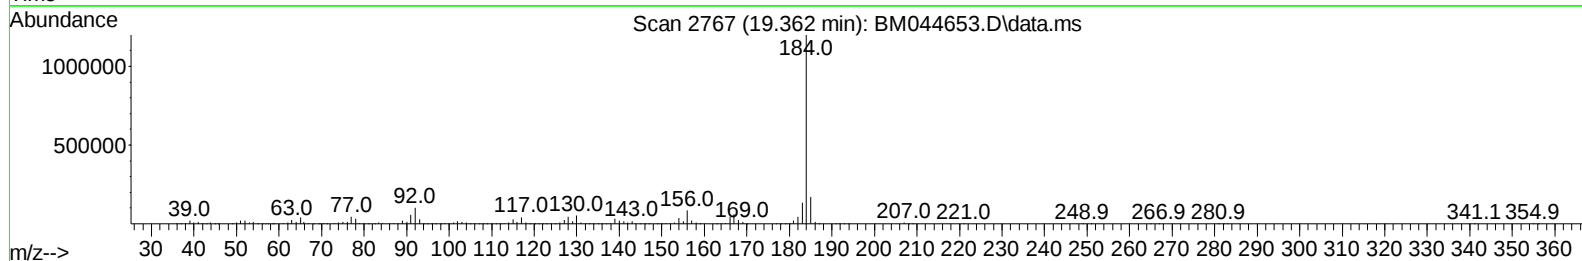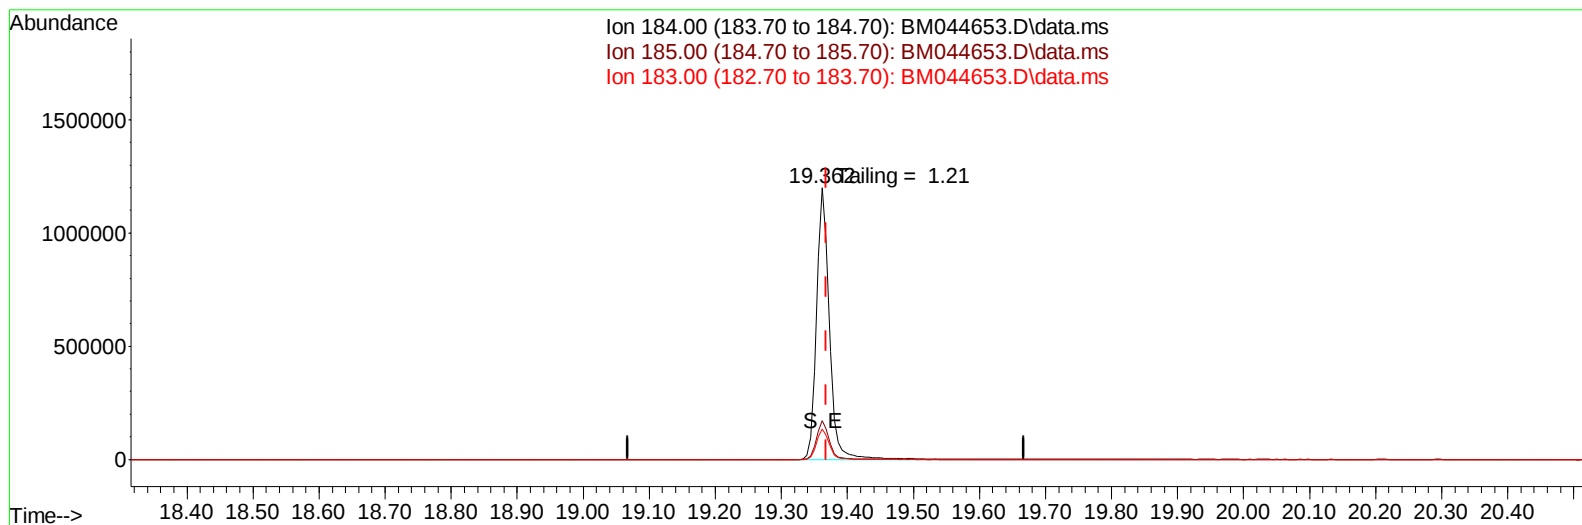

TIC: BM044653.D\data.ms

(77) Benzidine

19.362min (-0.006) 0.00 ng

response 1592721

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.20
183.00	10.90	11.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/18/2024	BNA_M	<u>BM044653.D</u>
Compound Name	Response	Retention Time
DDT	796654	20.597
DDD	12284	20.203
DDE	1303	19.645
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13587	810241	1.68

Instrument :
BNA_M
ClientSampleId :
DFTPP