


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032521\
 Data File : BM029206.D
 Acq On : 24 Mar 2021 16:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 25 02:53:41 2021

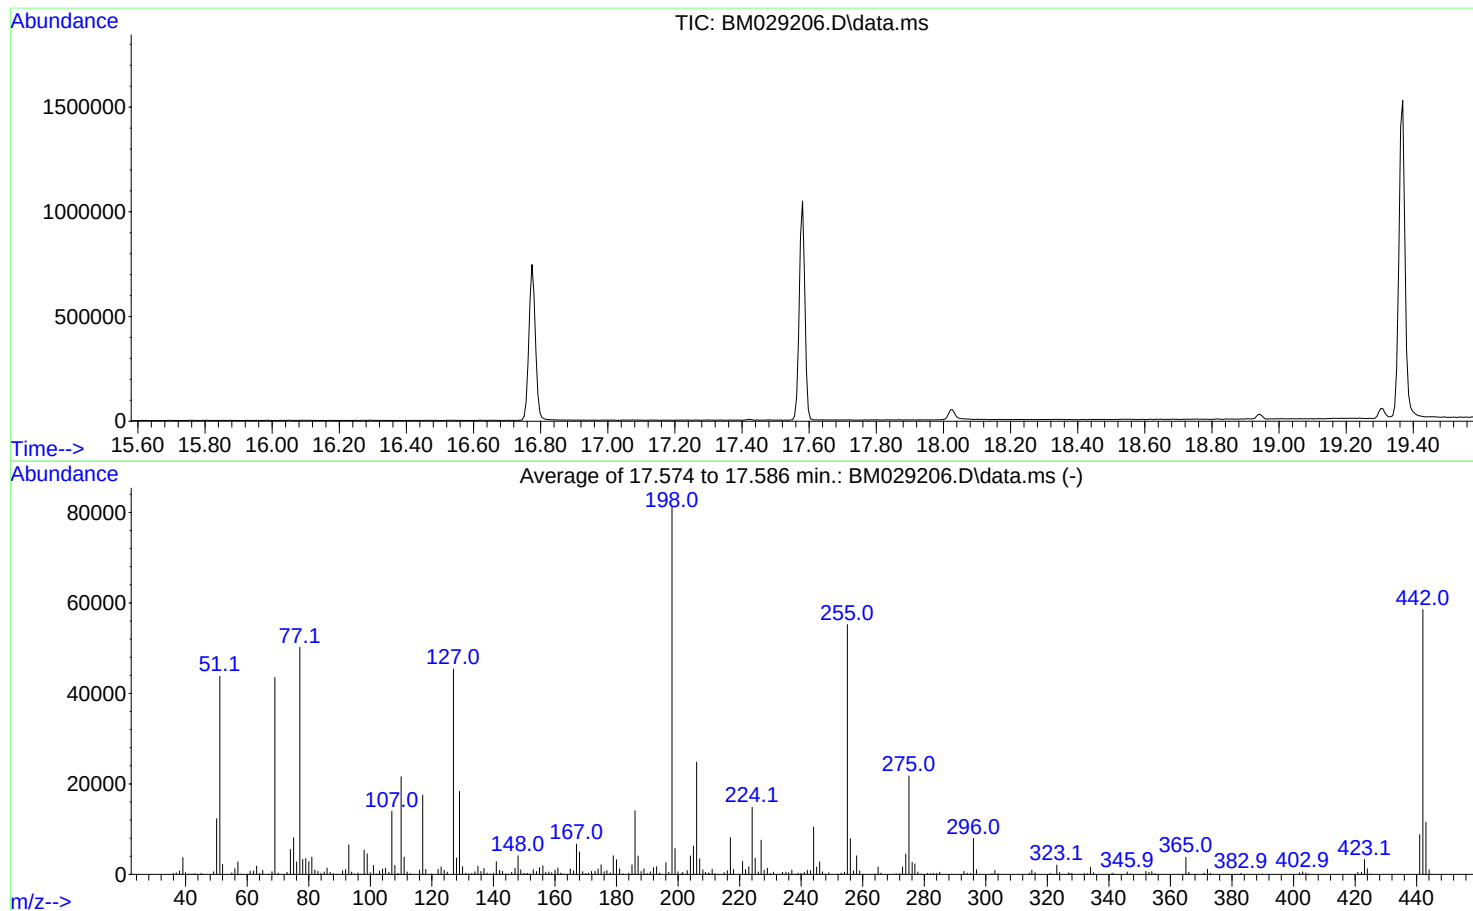




AutoFind: Scans 2497, 2498, 2499; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.8	43768	PASS
68	69	0.00	2	1.4	616	PASS
69	198	0.00	100	53.5	43539	PASS
70	69	0.00	2	0.6	271	PASS
127	198	10	80	55.8	45347	PASS
197	198	0.00	2	0.6	466	PASS
198	198	100	100	100.0	81312	PASS
199	198	5	9	7.0	5681	PASS
275	198	10	60	26.7	21744	PASS
365	198	1	100	4.7	3794	PASS
441	198	0.01	100	10.8	8769	PASS
442	442	50	100	100.0	58544	PASS
443	442	15	24	19.7	11530	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032521\
 Data File : BM029206.D
 Acq On : 24 Mar 2021 16:03
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 25 06:12:04 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 25 02:53:41 2021
 Response via : Initial Calibration

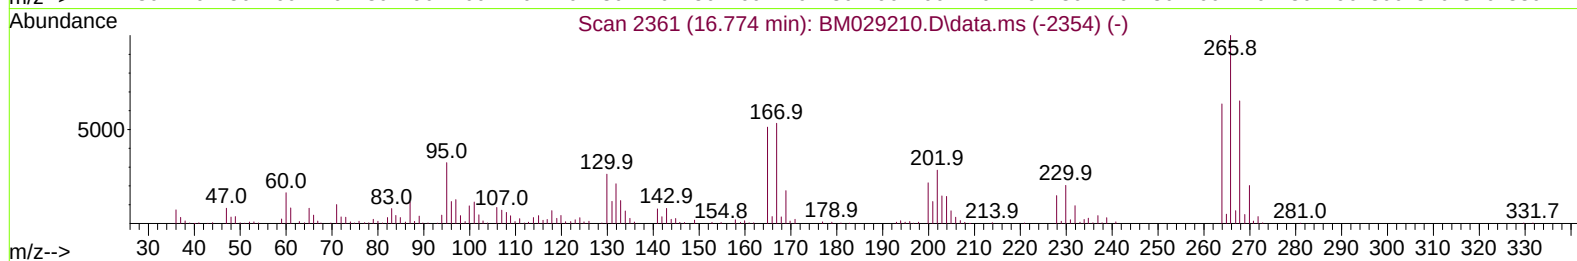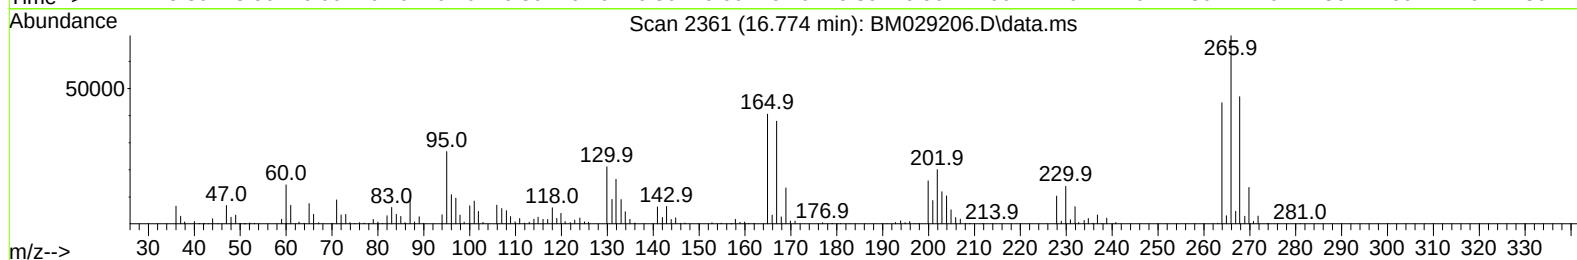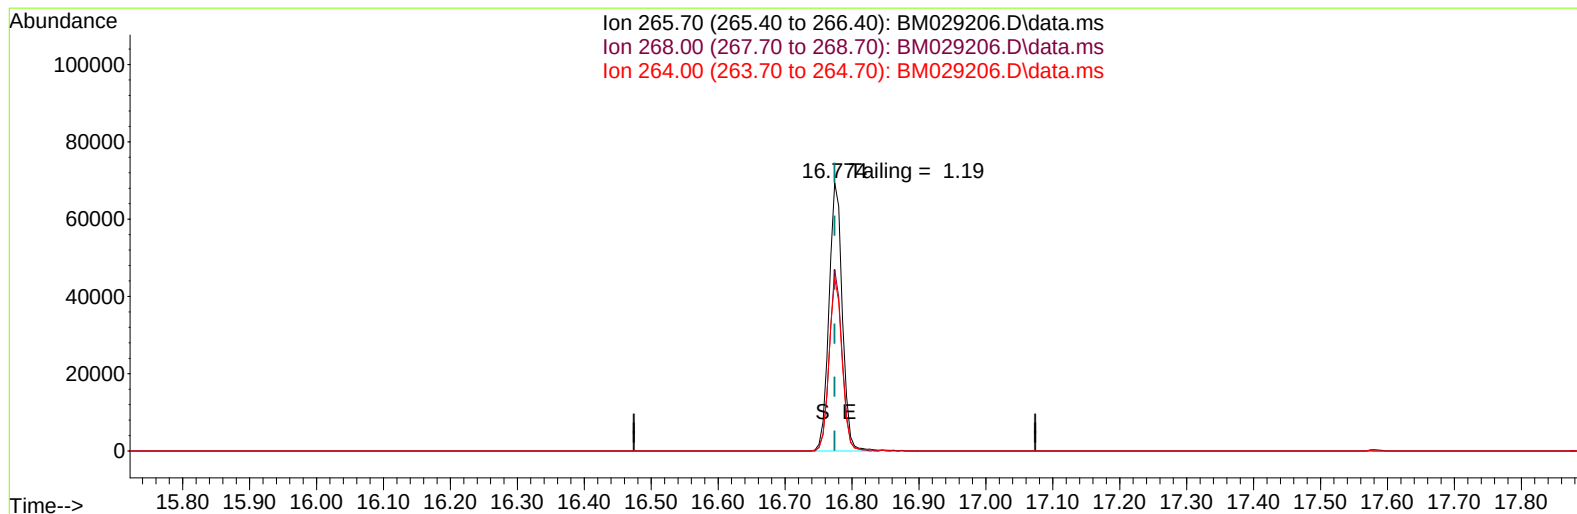

TIC: BM029206.D\data.ms

(70) Pentachlorophenol (C)

16.774min (+ 0.000) 0.00 ng




response 96623

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	67.64
264.00	63.60	64.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032521\
Data File : BM029206.D
Acq On : 24 Mar 2021 16:03
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 25 06:12:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 02:53:41 2021
Response via : Initial Calibration

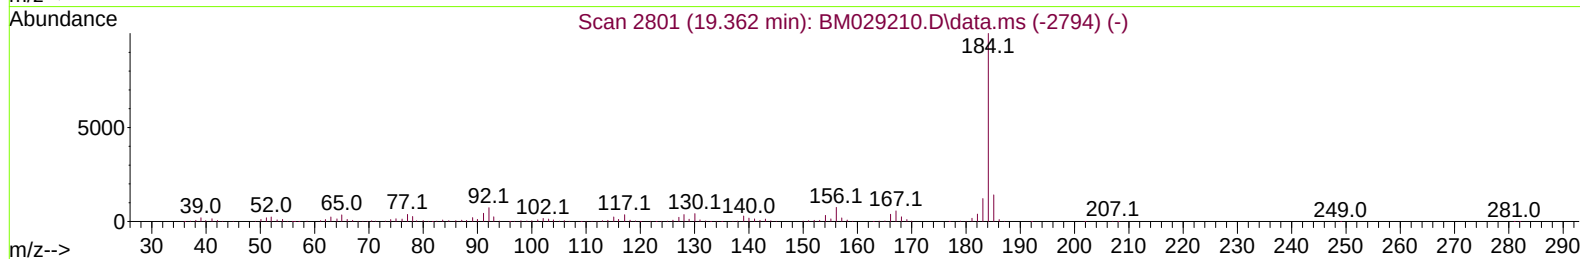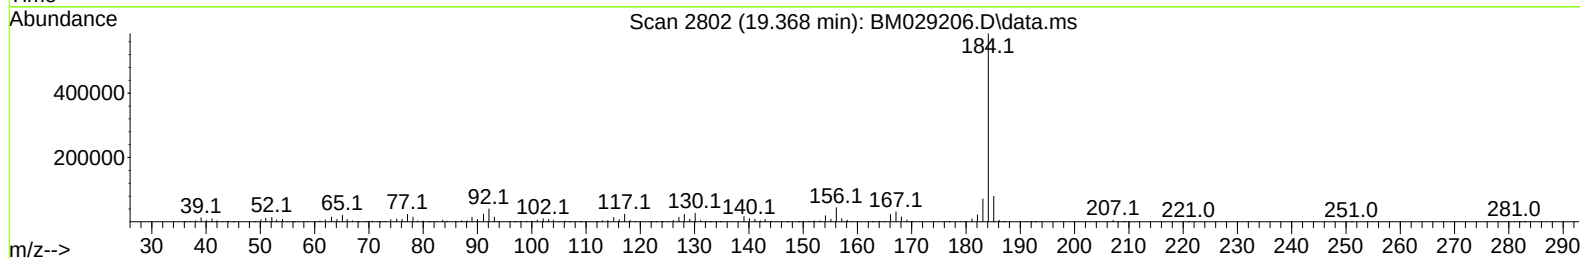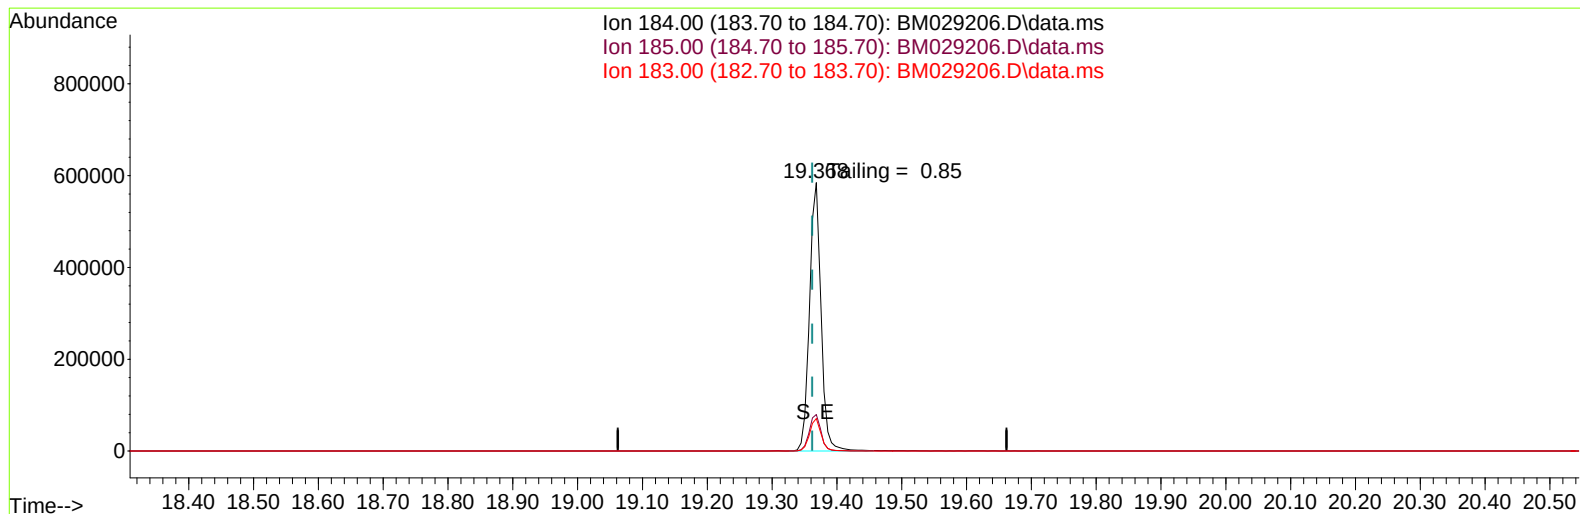

TIC: BM029206.D\data.ms

(77) Benzidine

19.368min (+ 0.006) 0.00 ng

response 723941

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.59
183.00	12.20	12.12
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/25/2021	BNA_M	<u>BM029206.D</u>
Compound Name	Response	Retention Time
DDT	320733	20.603
DDD	1282	20.221
DDE	318	19.662
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1600	322333	0.50