
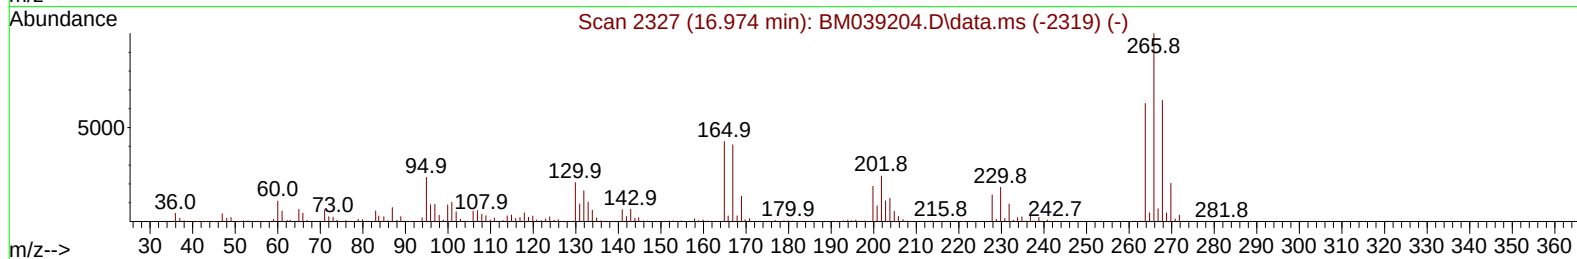
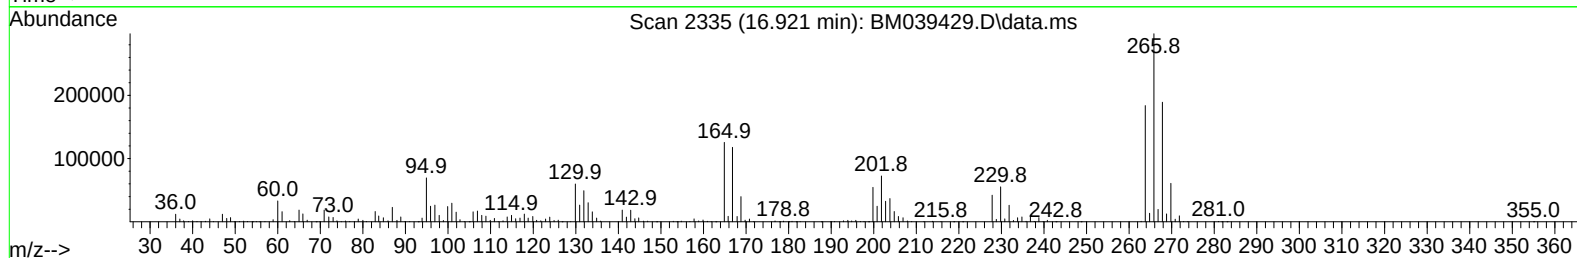


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041423\
Data File : BM039429.D
Acq On : 14 Apr 2023 11:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 16:55:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 14:49:28 2023
Response via : Initial Calibration

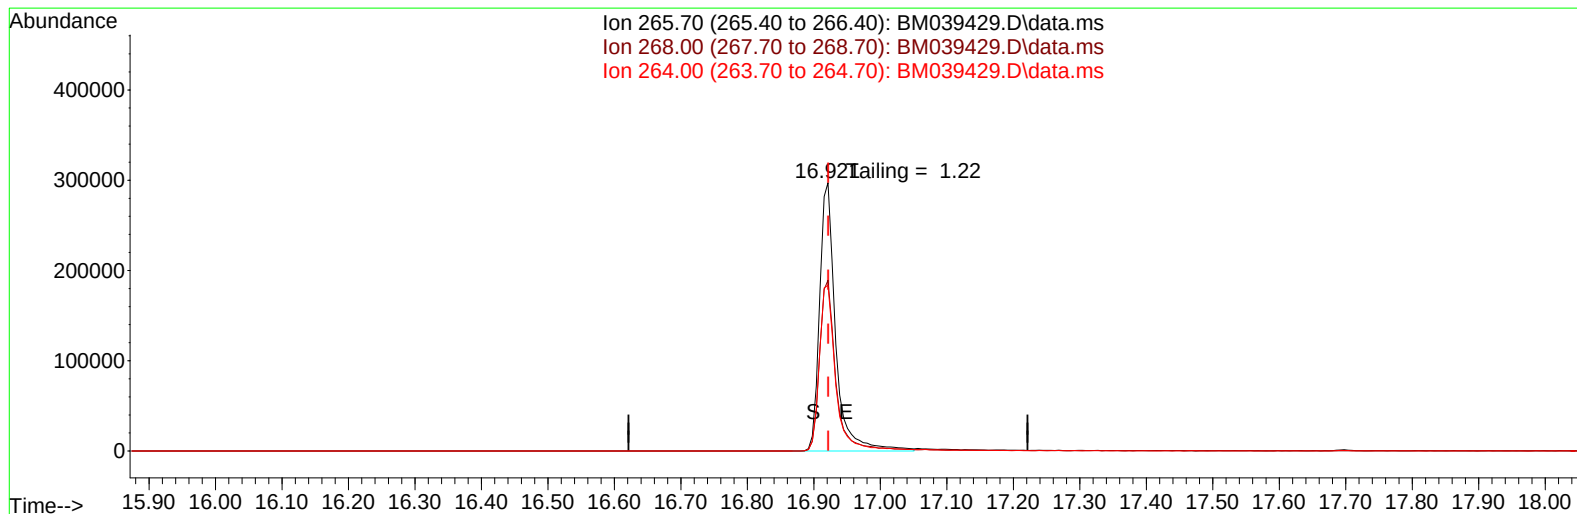

TIC: BM039429.D\data.ms

(70) Pentachlorophenol (C)




16.921min (-0.000) 424911.39 ng

response 501272

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.60
264.00	62.80	61.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041423\
Data File : BM039429.D
Acq On : 14 Apr 2023 11:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 14 16:55:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 14:49:28 2023
Response via : Initial Calibration

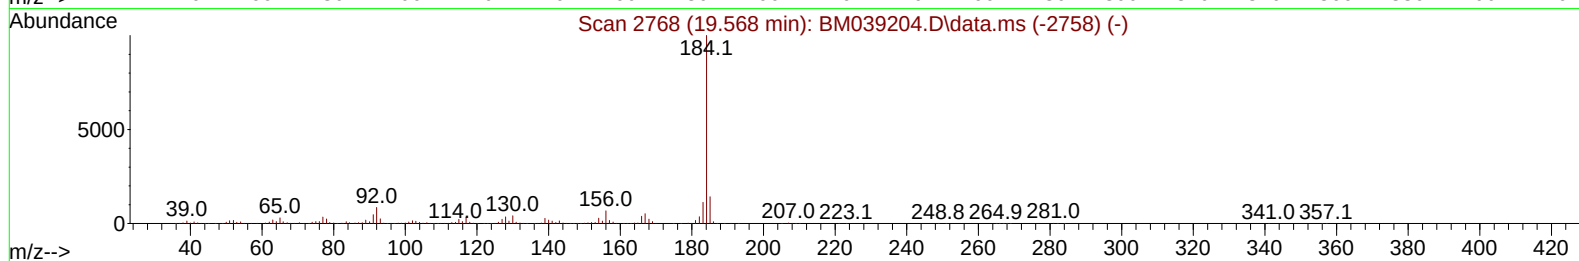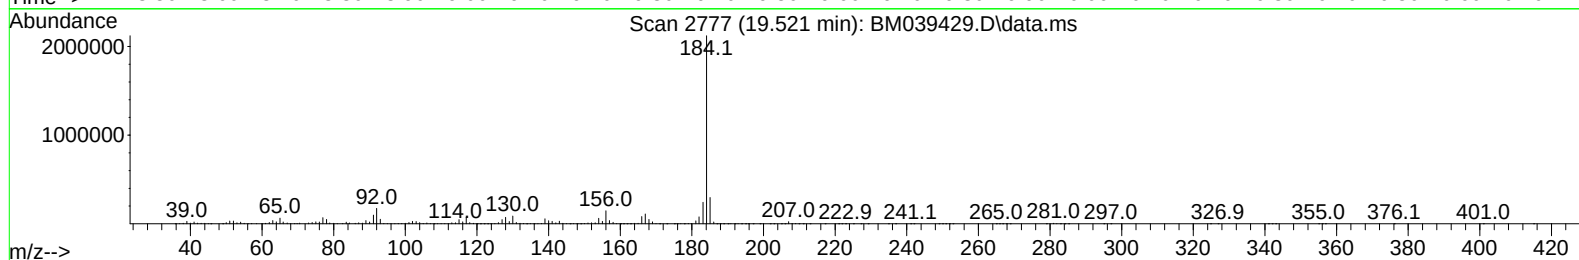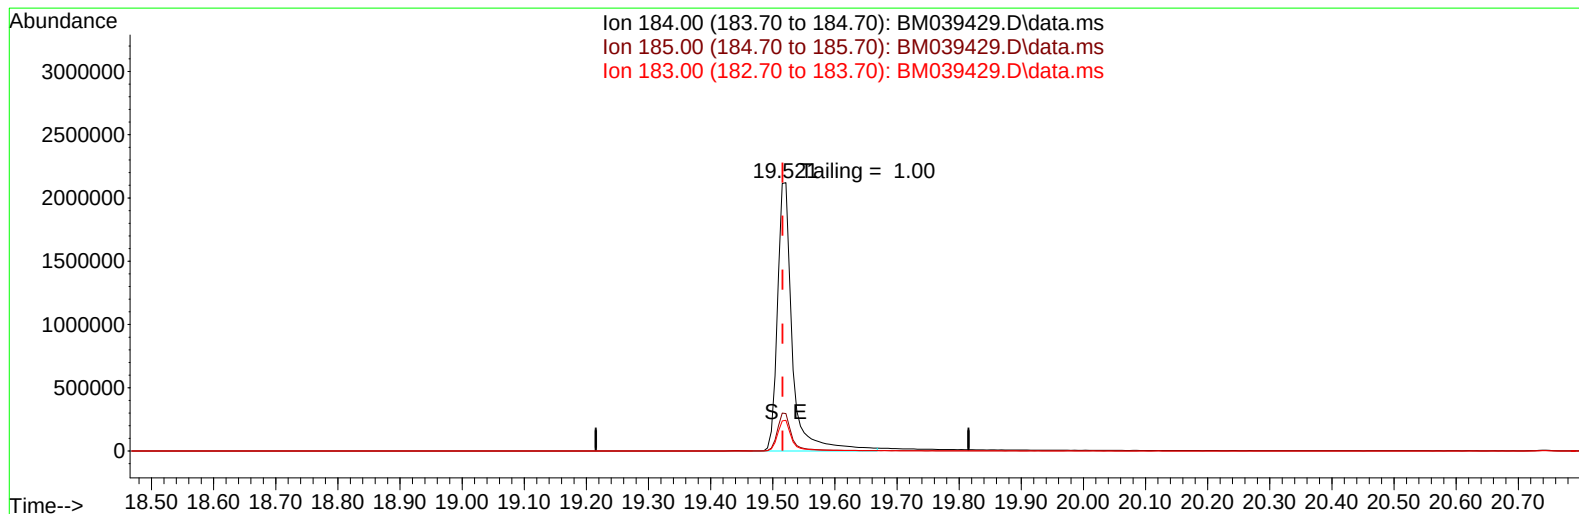

TIC: BM039429.D\data.ms

(77) Benzidine**19.521min (+ 0.006) 61981.07 ng****response 3665308**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.96
183.00	11.20	11.46
0.00	0.00	0.00