
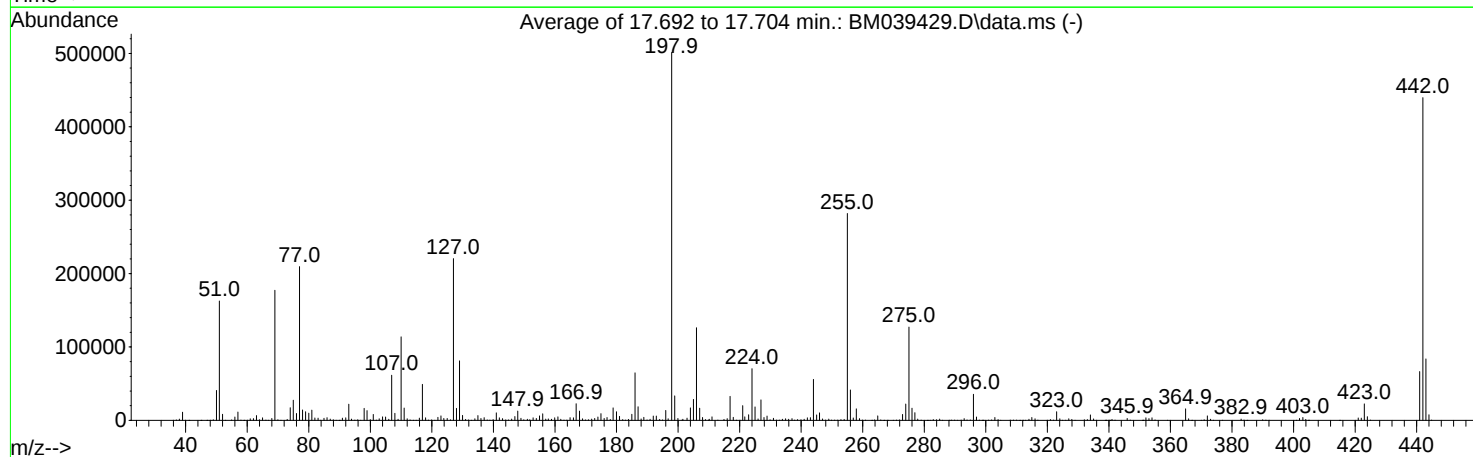


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041423\
Data File : BM039429.D
Acq On : 14 Apr 2023 11:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 14 17:54:10 2023

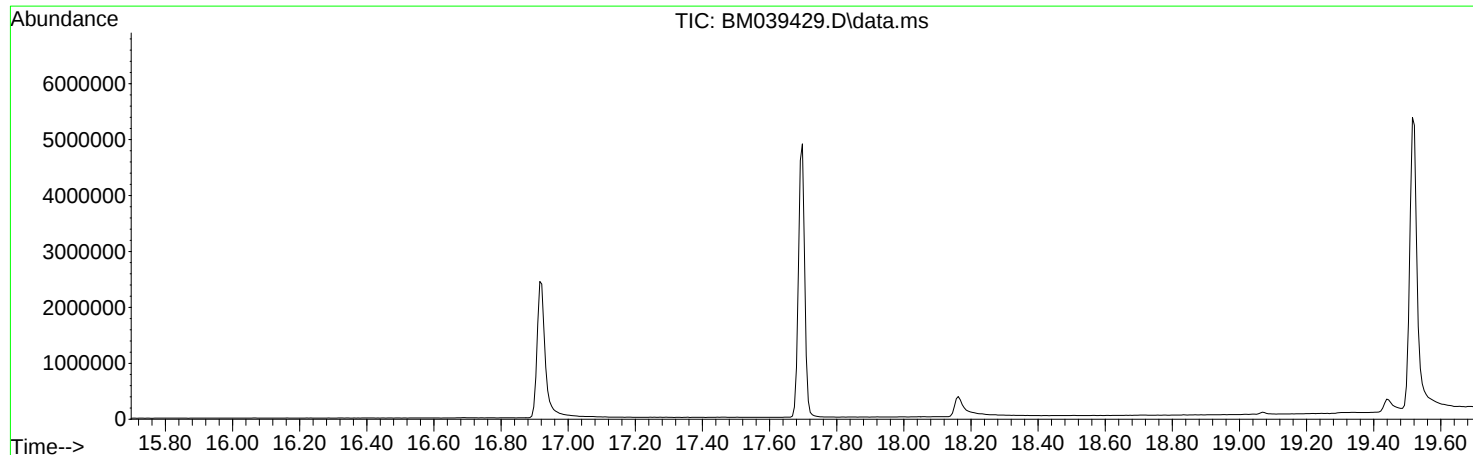




AutoFind: Scans 2466, 2467, 2468; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.4	162582	PASS
68	69	0.00	2	1.5	2738	PASS
69	198	0.00	100	35.4	177253	PASS
70	69	0.00	2	0.5	866	PASS
127	198	10	80	44.0	220480	PASS
197	198	0.00	2	0.4	2109	PASS
198	198	100	100	100.0	501248	PASS
199	198	5	9	6.7	33477	PASS
275	198	10	60	25.4	127115	PASS
365	198	1	100	3.1	15751	PASS
441	198	0.01	100	13.2	66403	PASS
442	442	50	100	100.0	439659	PASS
443	442	15	24	19.1	83784	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041423\
Data File : BM039429.D
Acq On : 14 Apr 2023 11:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 14 16:55:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 14:49:28 2023
Response via : Initial Calibration

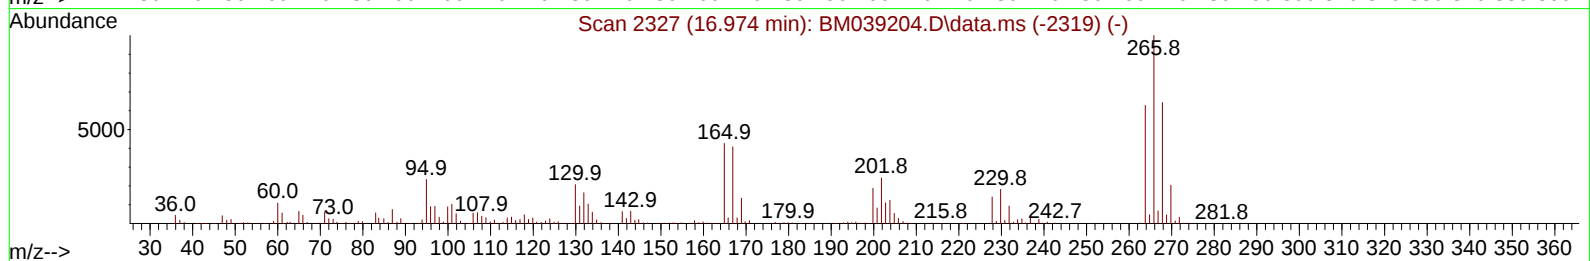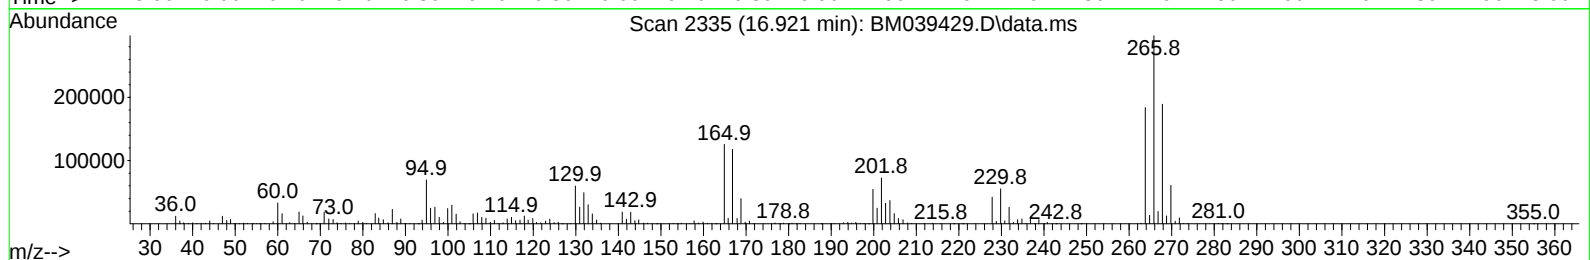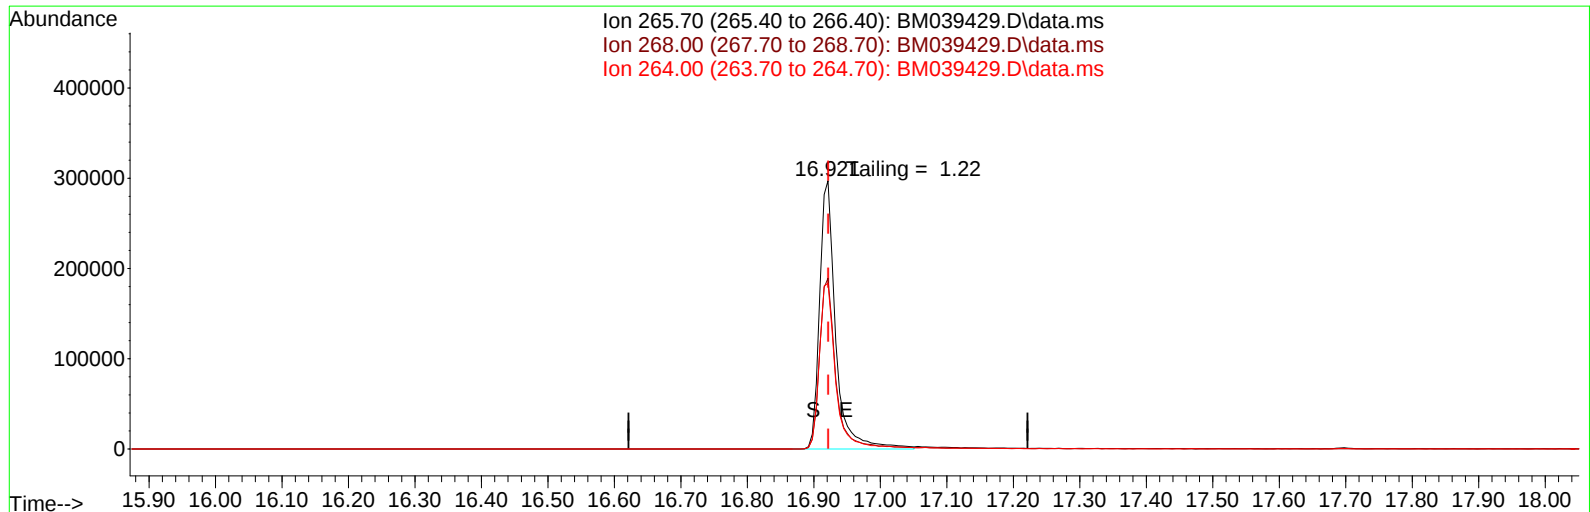

TIC: BM039429.D\data.ms

(70) Pentachlorophenol (C)

16.921min (-0.000) 424911.39 ng




response 501272

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.30	63.60
264.00	62.80	61.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041423\
Data File : BM039429.D
Acq On : 14 Apr 2023 11:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Apr 14 16:55:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM032923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 14 14:49:28 2023
Response via : Initial Calibration

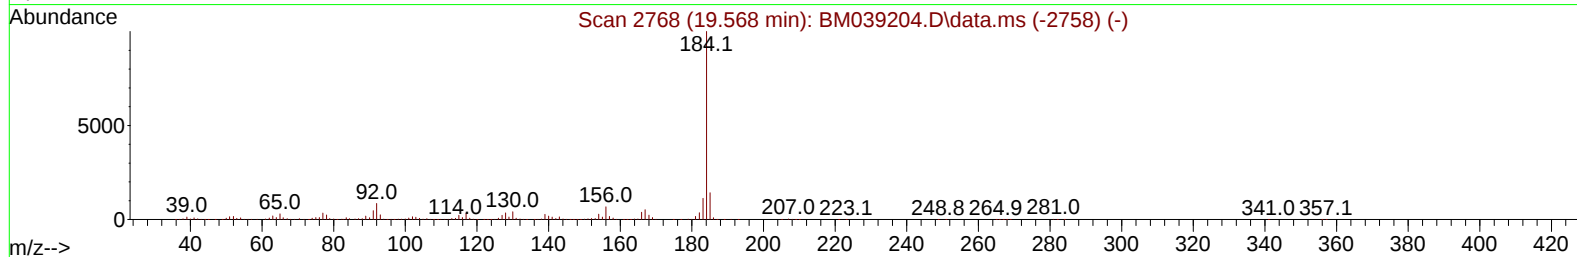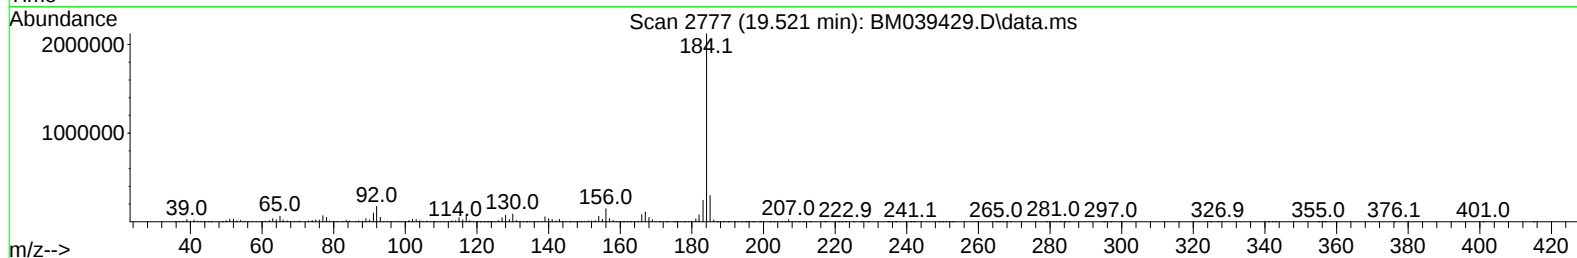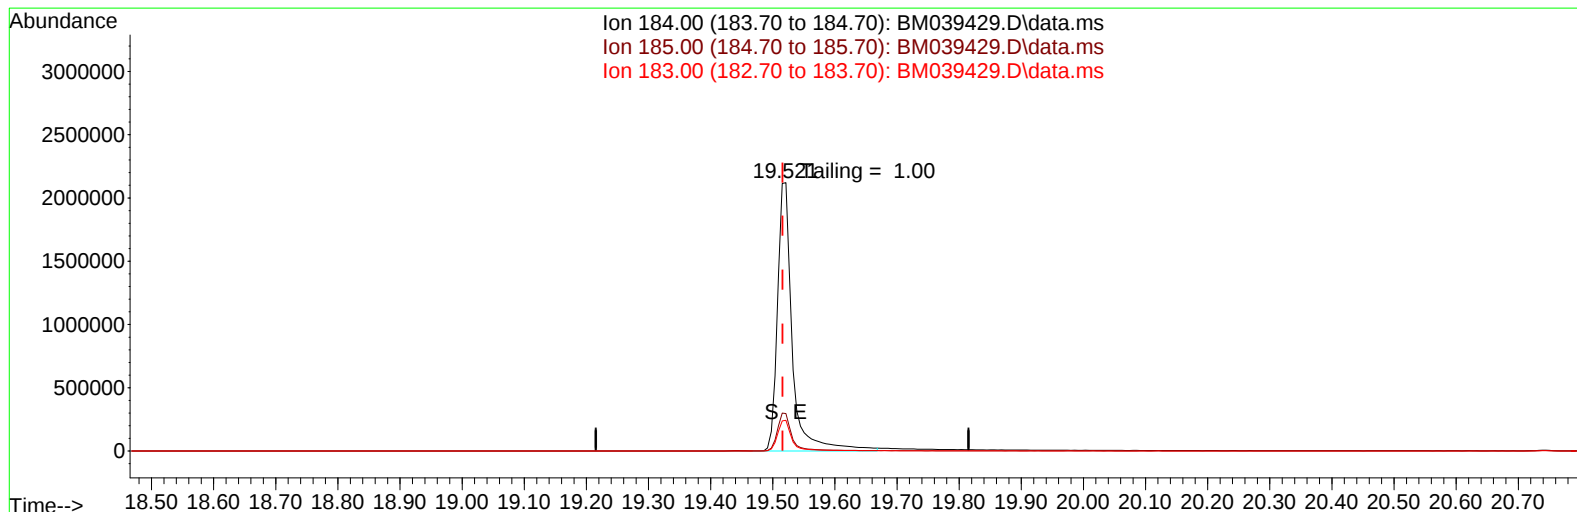

TIC: BM039429.D\data.ms

(77) Benzidine

19.521min (+ 0.006) 61981.07 ng

response 3665308

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.96
183.00	11.20	11.46
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/14/2023	BNA_M	<u>BM039429.D</u>
Compound Name	Response	Retention Time
DDT	1661590	20.745
DDD	26236	20.35
DDE	1608	19.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
27844	1689434	1.65

Instrument :
BNA_M
ClientSampleId :
DFTPP