
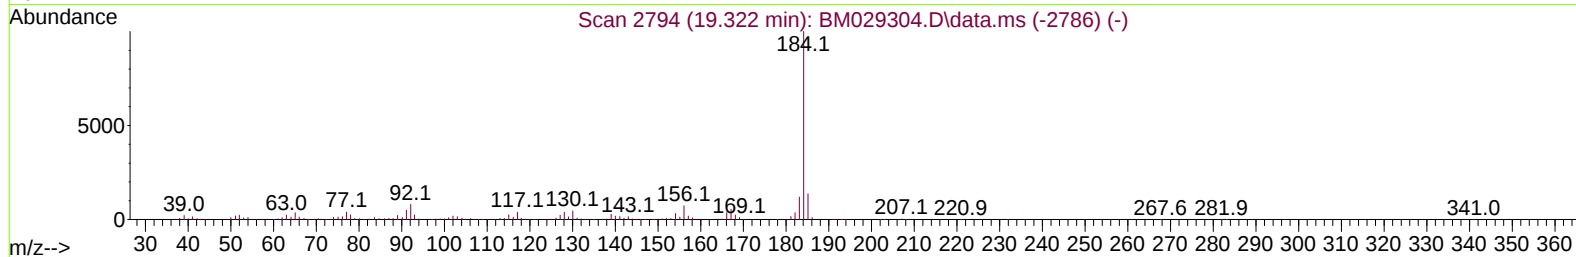
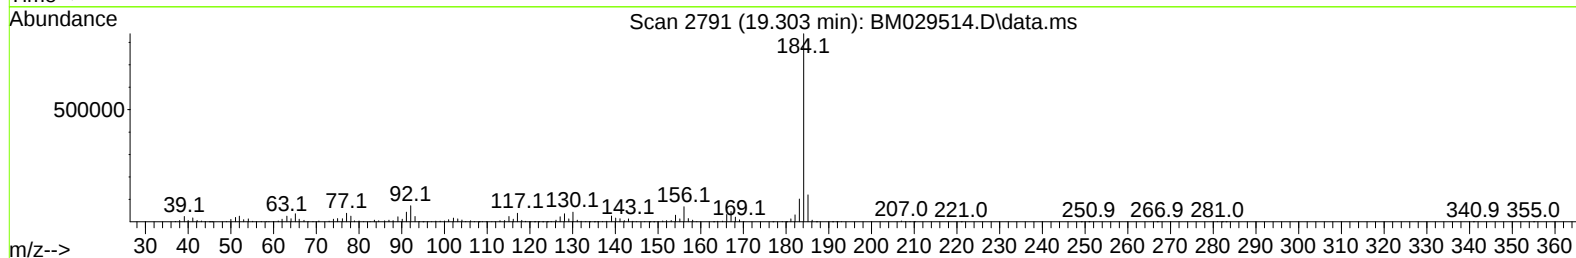


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041621\
 Data File : BM029514.D
 Acq On : 16 Apr 2021 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 08:14:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 11:56:50 2021
 Response via : Initial Calibration

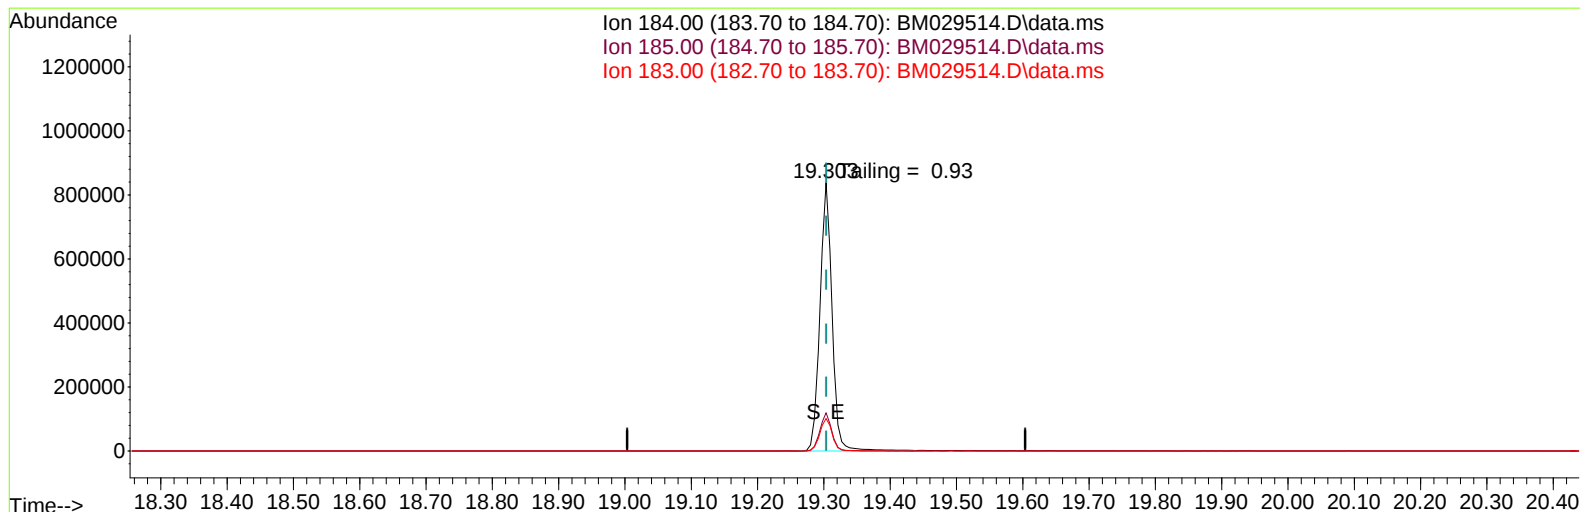

TIC: BM029514.D\data.ms

(77) Benzidine




19.303min (-0.000) 0.00 ng

response 1067176

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.30
183.00	12.20	12.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041621\
Data File : BM029514.D
Acq On : 16 Apr 2021 10:12
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 17 08:14:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 16 11:56:50 2021
Response via : Initial Calibration

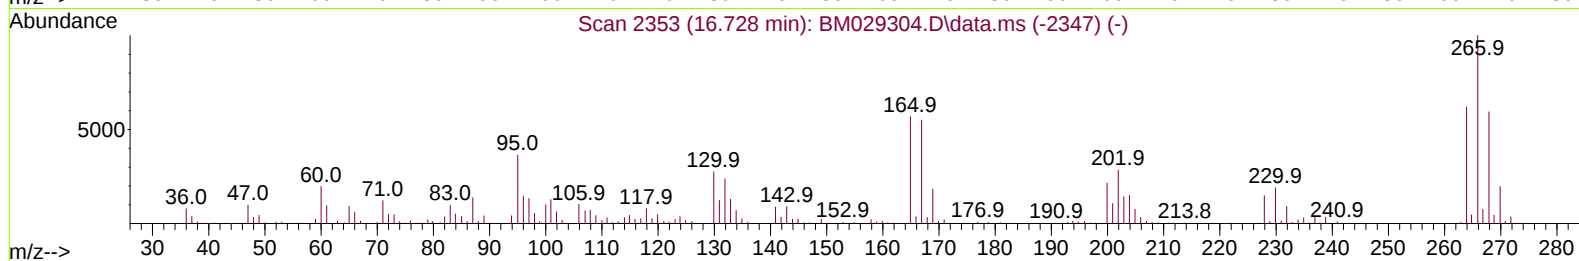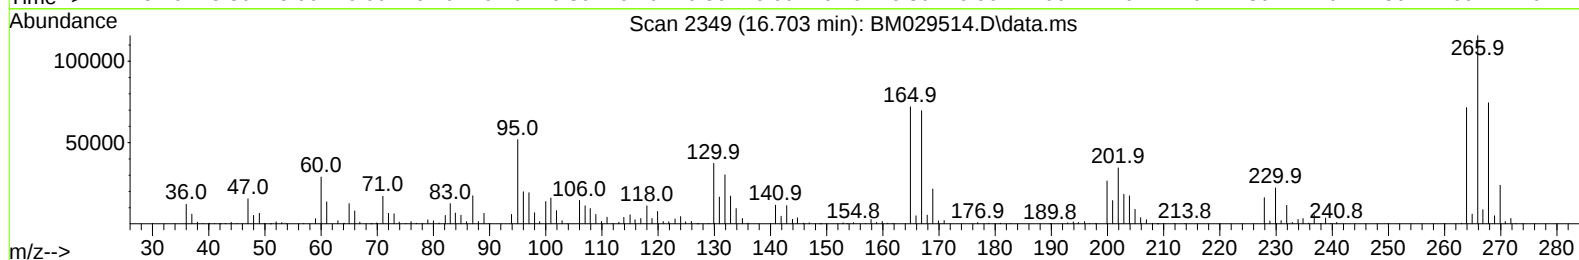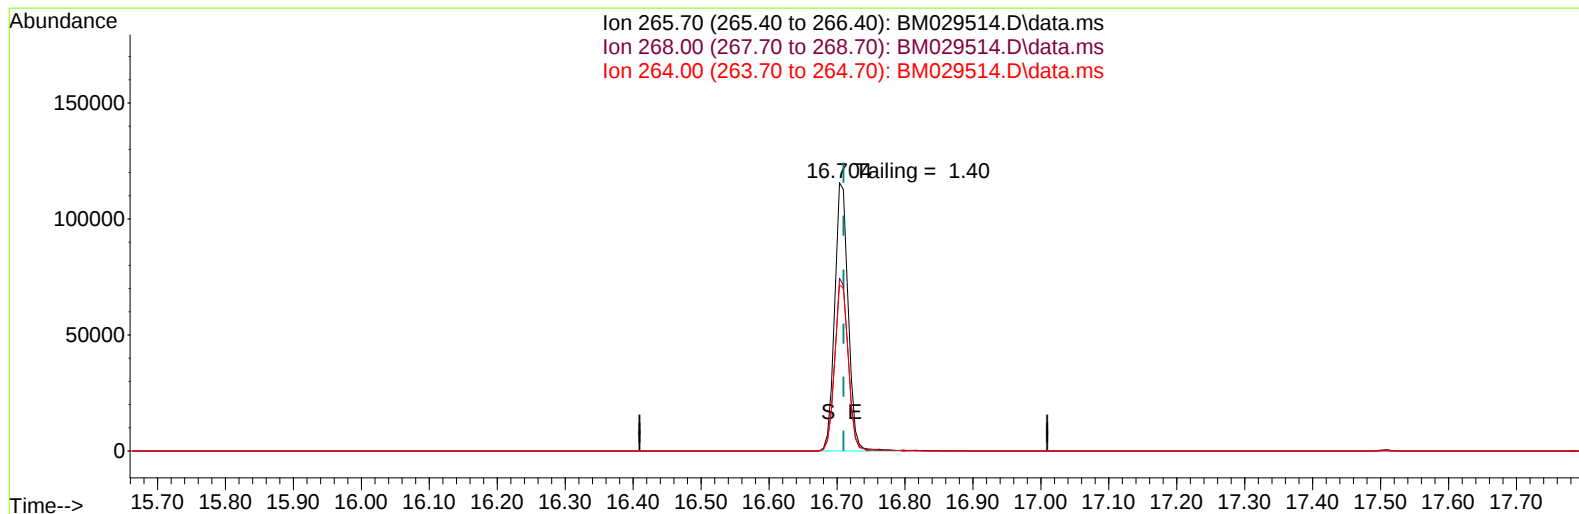

TIC: BM029514.D\data.ms

(70) Pentachlorophenol (C)

16.703min (-0.006) 0.00 ng

response 160297

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	64.43
264.00	63.60	61.87
0.00	0.00	0.00