

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041621\
 Data File : BM029516.D
 Acq On : 16 Apr 2021 11:27
 Operator : CG/JU
 Sample : PB135697BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB135697BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM029516.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.922	3	6	17	rVB	75330	97552	2.02%	0.359%
2	5.275	399	406	422	rBV	2512647	3523443	72.87%	12.962%
3	6.851	666	674	694	rBV	2376508	3670245	75.91%	13.502%
4	7.675	807	814	823	rBV	421689	664223	13.74%	2.444%
5	8.828	1002	1010	1030	rBV	1411684	2308692	47.75%	8.493%
6	10.451	1278	1286	1297	rBV	496532	853753	17.66%	3.141%
7	12.933	1701	1708	1722	rBV	3136355	4408915	91.18%	16.220%
8	14.310	1936	1942	1954	rBV2	665930	995662	20.59%	3.663%
9	15.804	2189	2196	2206	rBV	2217437	3034309	62.75%	11.163%
10	17.056	2403	2409	2419	rBV	698718	997107	20.62%	3.668%
11	19.686	2850	2856	2865	rBV	4305771	4835288	100.00%	17.788%
12	21.233	3114	3119	3126	rBV	760433	909612	18.81%	3.346%
13	23.438	3488	3494	3504	rVB2	490983	883778	18.28%	3.251%




Sum of corrected areas: 27182579

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041621\
Data File : BM029516.D
Acq On : 16 Apr 2021 11:27
Operator : CG/JU
Sample : PB135697BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135697BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

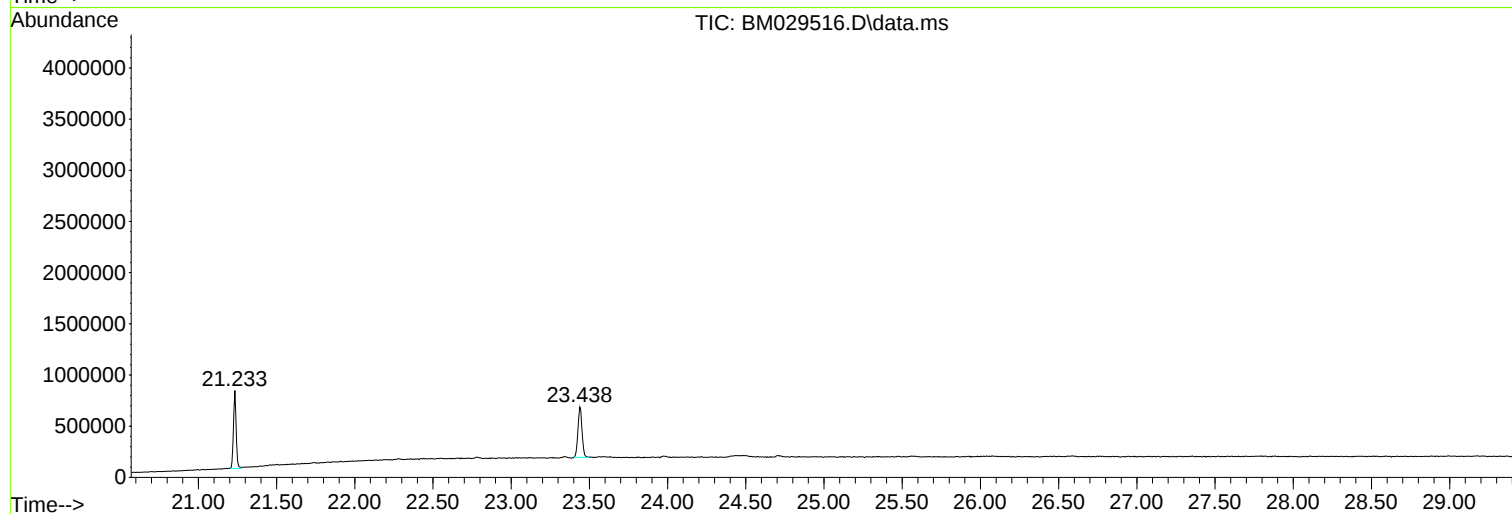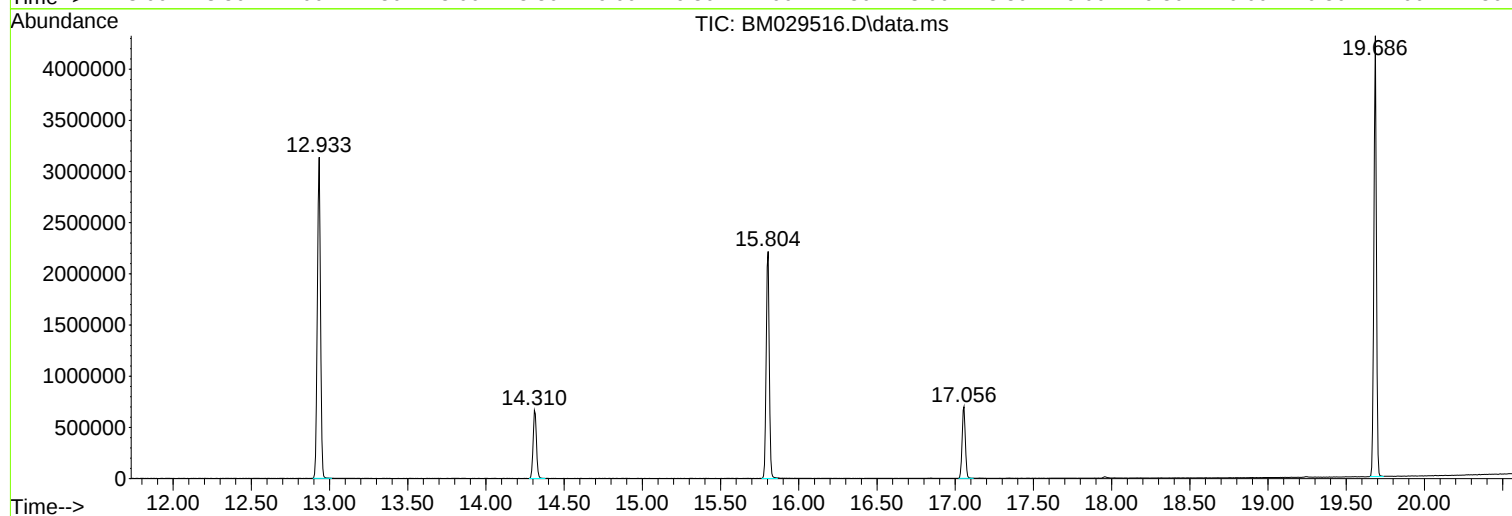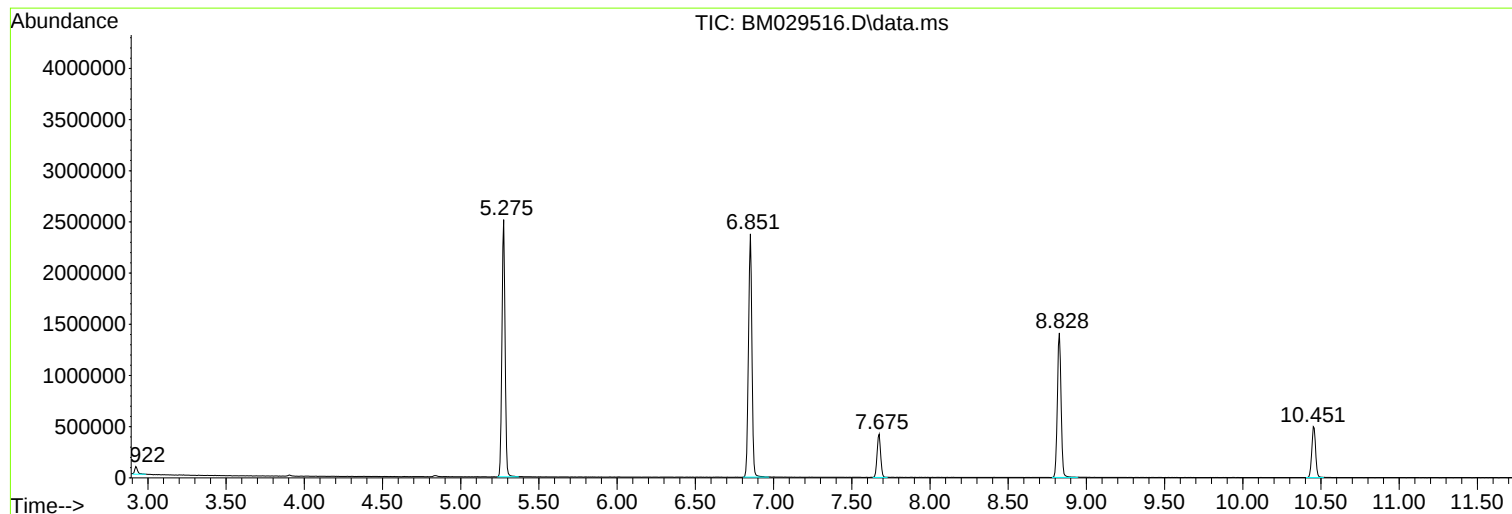

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041621\
Data File : BM029516.D
Acq On : 16 Apr 2021 11:27
Operator : CG/JU
Sample : PB135697BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135697BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.922	2.94 ng	97552	1,4-Dichlorobenzene-d4	7.675

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			Butanoic acid, 2-hydroxy-2-methyl-	132	C6H12O3	032793-34-3	43
3			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	40
4			Myo-Inositol, 4-C-methyl-	194	C7H14O6	000472-95-7	33
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	27

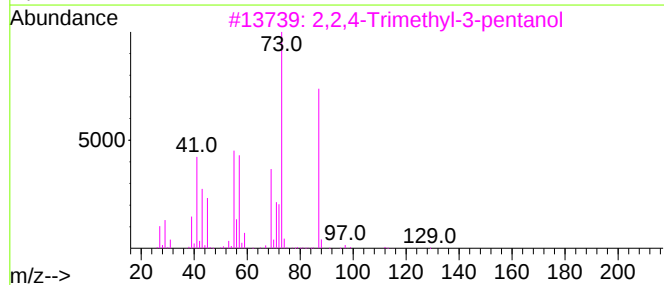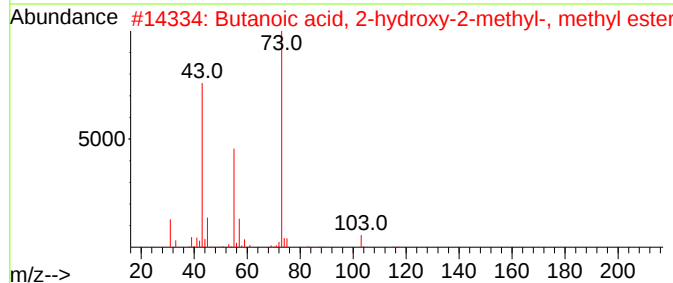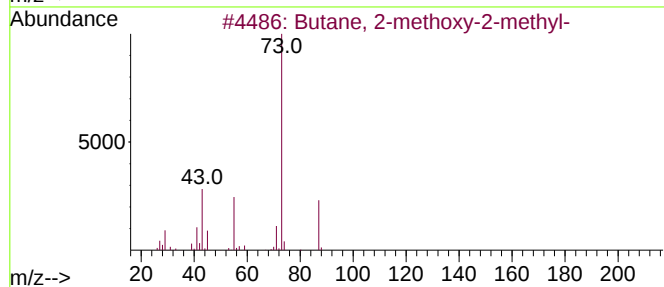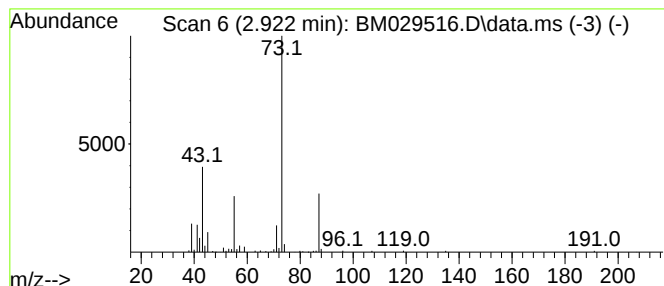

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041621\
Data File : BM029516.D
Acq On : 16 Apr 2021 11:27
Operator : CG/JU
Sample : PB135697BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB135697BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.922	2.9	ng	97552	1	7.675	664223	20.0