
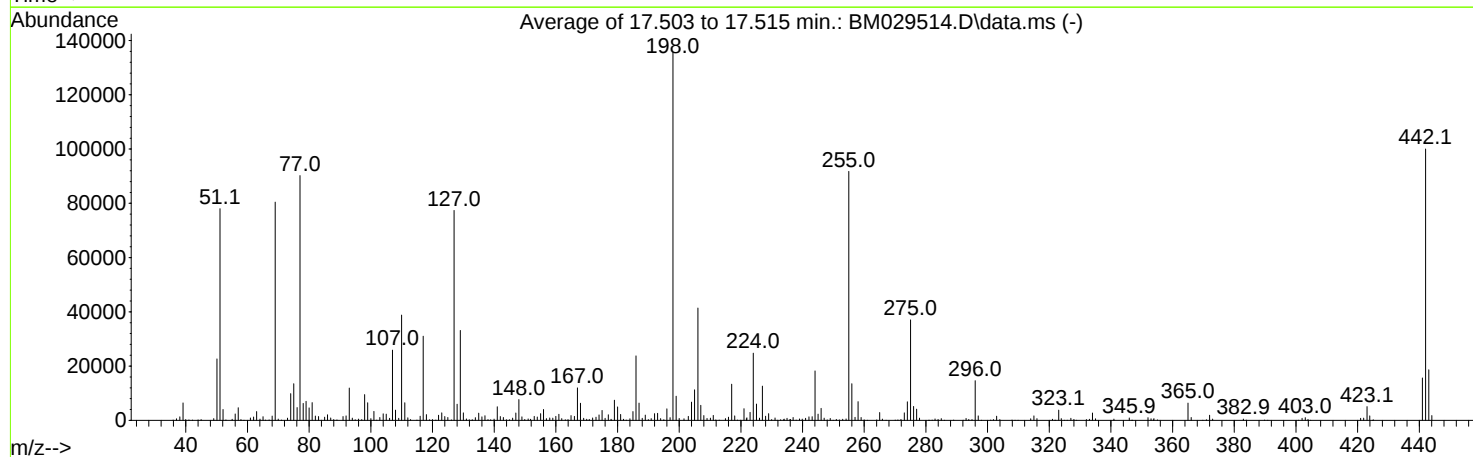


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041621\
 Data File : BM029514.D
 Acq On : 16 Apr 2021 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 16 11:56:50 2021

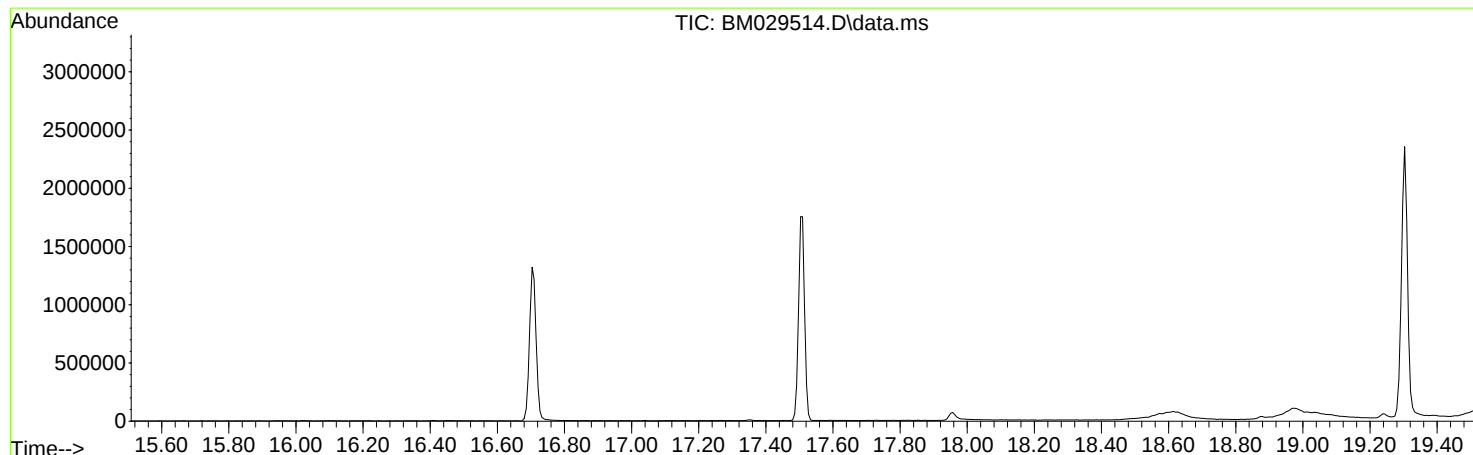

AutoFind: Scans 2485, 2486, 2487; Background Corrected with Scan 2478

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.5	78011	PASS
68	69	0.00	2	2.0	1581	PASS
69	198	0.00	100	59.3	80451	PASS
70	69	0.00	2	0.6	452	PASS
127	198	10	80	57.1	77381	PASS
197	198	0.00	2	0.8	1032	PASS
198	198	100	100	100.0	135587	PASS
199	198	5	9	6.6	8932	PASS
275	198	10	60	27.3	37061	PASS
365	198	1	100	4.7	6354	PASS
441	198	0.01	100	11.5	15615	PASS
442	442	50	100	100.0	100021	PASS
443	442	15	24	18.6	18622	PASS

Instrument :
BNA_M
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/16/2021	BNA_M	<u>BM029514.D</u>
Compound Name	Response	Retention Time
DDT	548936	20.539
DDD	15042	20.097
DDE	849	19.586
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15891	564827	2.81

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041621\
 Data File : BM029514.D
 Acq On : 16 Apr 2021 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 17 08:14:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 11:56:50 2021
 Response via : Initial Calibration

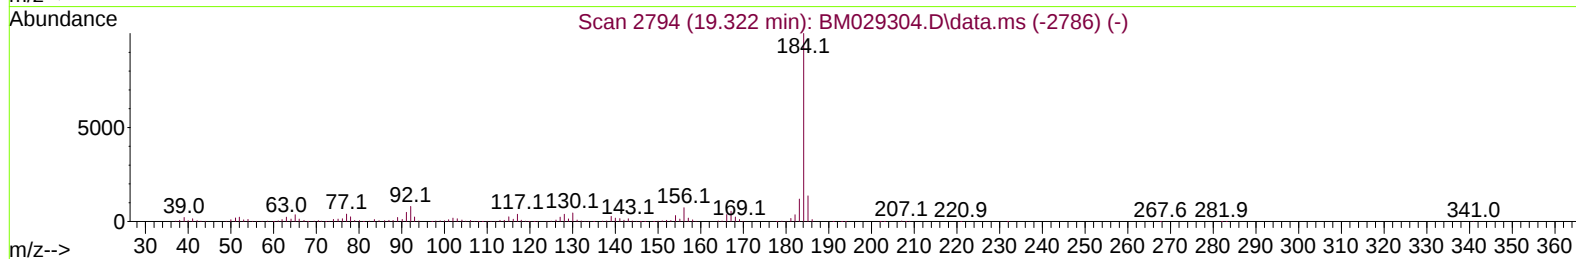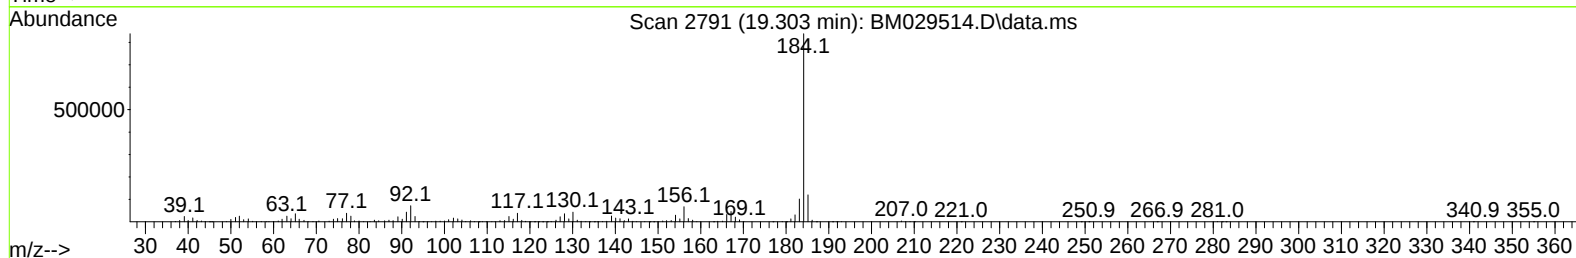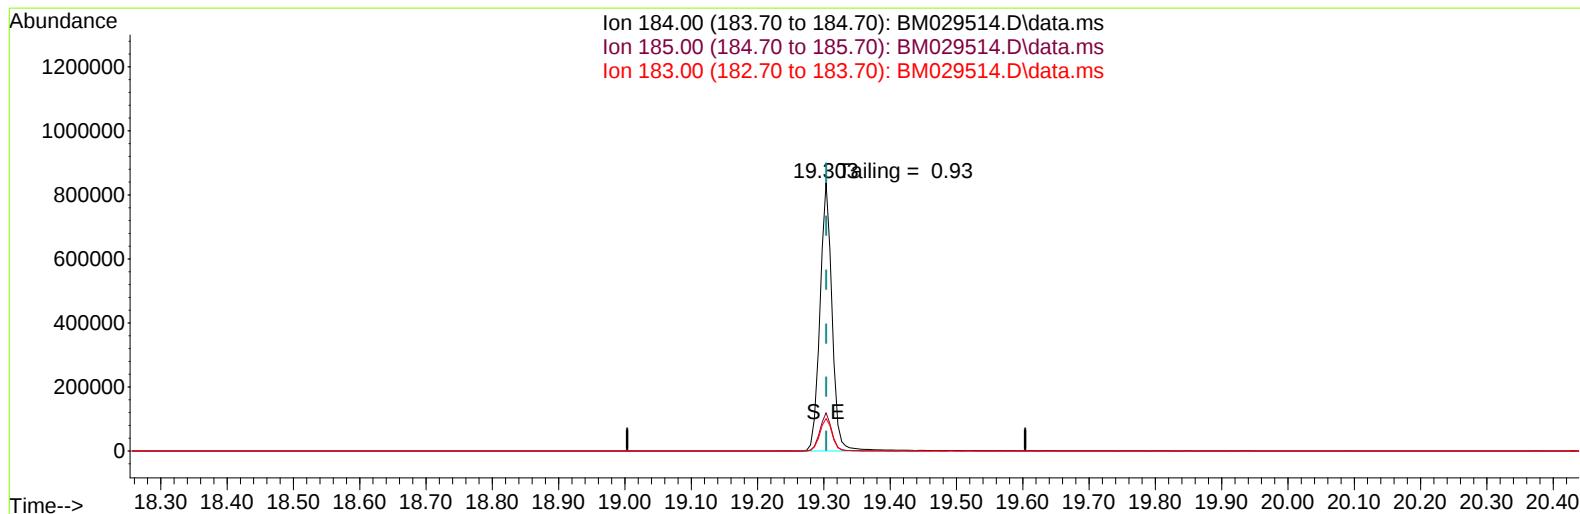

TIC: BM029514.D\data.ms

(77) Benzidine

19.303min (-0.000) 0.00 ng




response 1067176

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.30
183.00	12.20	12.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM041621\
 Data File : BM029514.D
 Acq On : 16 Apr 2021 10:12
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 17 08:14:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM040121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 16 11:56:50 2021
 Response via : Initial Calibration

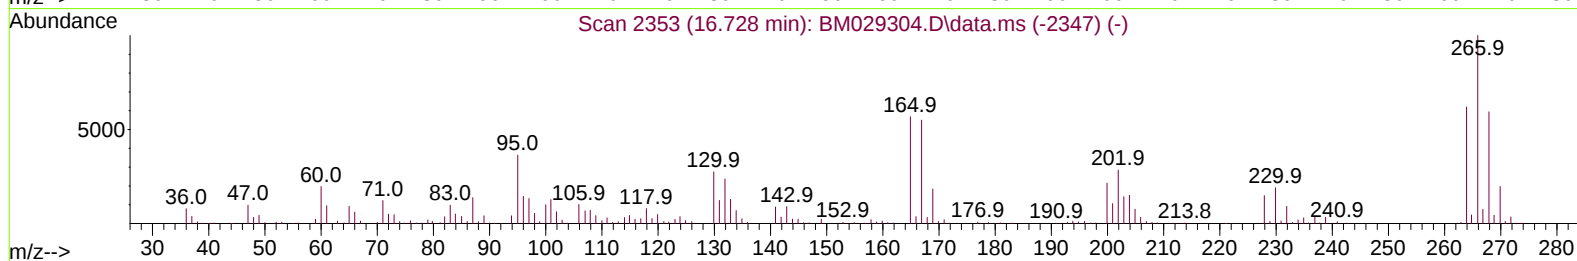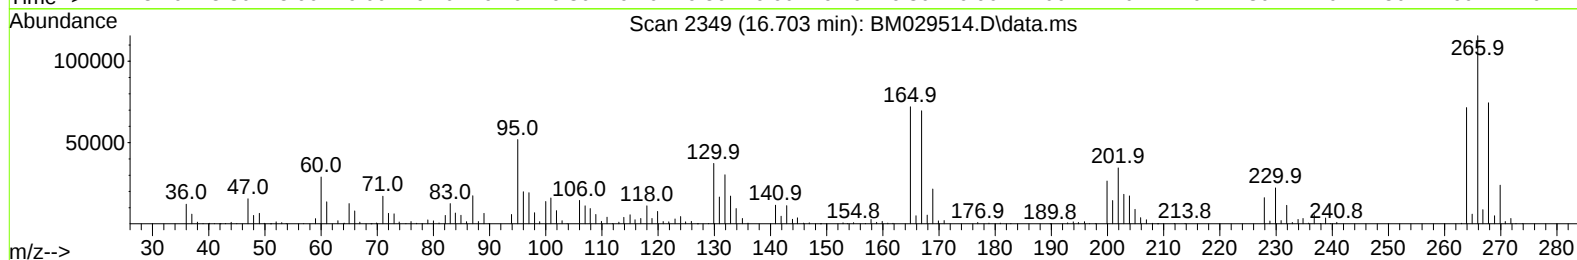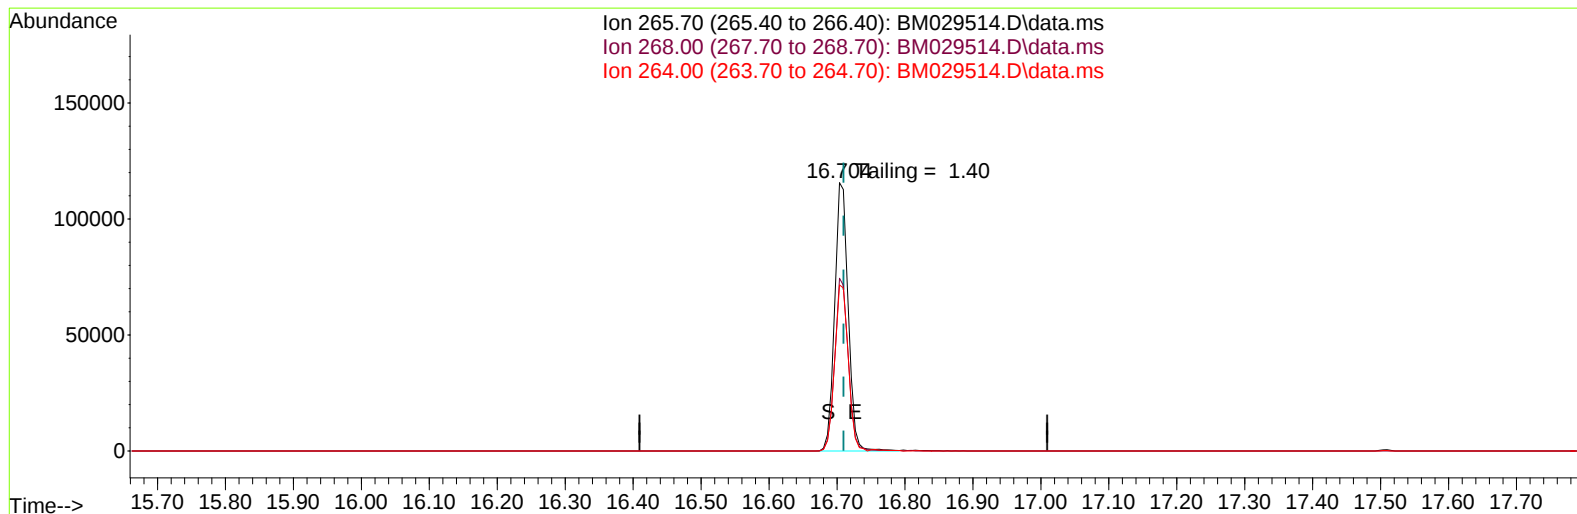

TIC: BM029514.D\data.ms

(70) Pentachlorophenol (C)

16.703min (-0.006) 0.00 ng

response 160297

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.20	64.43
264.00	63.60	61.87
0.00	0.00	0.00