

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
 Data File : BM039611.D
 Acq On : 24 Apr 2023 11:44
 Operator : CG/JU
 Sample : 02462-01DL2 50X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0QG4DL2

Quant Time: Apr 25 00:12:45 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 00:18:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	174845	20.000	ng/ul	0.00
20) Naphthalene-d8	10.619	136	734544	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.471	164	440542	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.224	188	816822	20.000	ng/ul	0.00
79) Chrysene-d12	21.424	240	674084	20.000	ng/ul	0.00
88) Perylene-d12	23.782	264	746153	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.219	96	501	0.110	ng/uL	0.01
4) Pyridine-d5	3.631	84	286	0.022	ng/ul	0.00
7) Phenol-d5	0.000	99	0	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	7.125	67	71	0.007	ng/ul	-0.02
11) 2-Chlorophenol-d4	7.384	132	270	0.022	ng/ul	0.04
15) 4-Methylphenol-d8	8.707	113	121	0.009	ng/ul	0.16
21) Nitrobenzene-d5	9.048	128	196	0.033	ng/ul	0.06
24) 2-Nitrophenol-d4	9.760	143	284	0.043	ng/ul	0.05
28) 2,4-Dichlorophenol-d3	10.413	165	317	0.028	ng/ul	0.15
31) 4-Chloroaniline-d4	10.760	131	59	0.003	ng/ul	-0.02
46) Dimethylphthalate-d6	13.913	166	19256	0.542	ng/ul	0.02
49) Acenaphthylene-d8	14.171	160	21604	0.541	ng/ul	0.00
54) 4-Nitrophenol-d4	0.000	143	0	0.000	ng/ul	
60) Fluorene-d10	15.483	176	16537	0.568	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	0.000	200	0	0.000	ng/ul	
73) Anthracene-d10	17.224	188	816822	20.794	ng/ul	-0.10
81) Pyrene-d10	19.636	212	26926	0.601	ng/ul	0.01
92) Benzo(a)pyrene-d12	23.635	264	27489	0.682	ng/ul	0.00
Target Compounds						
					Qvalue	
71) Pentachlorophenol	16.889	266	185145	31.249	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039611.D
Acq On : 24 Apr 2023 11:44
Operator : CG/JU
Sample : 02462-01DL2 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0QG4DL2


Quant Time: Apr 25 00:12:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 00:18:16 2023
Response via : Initial Calibration

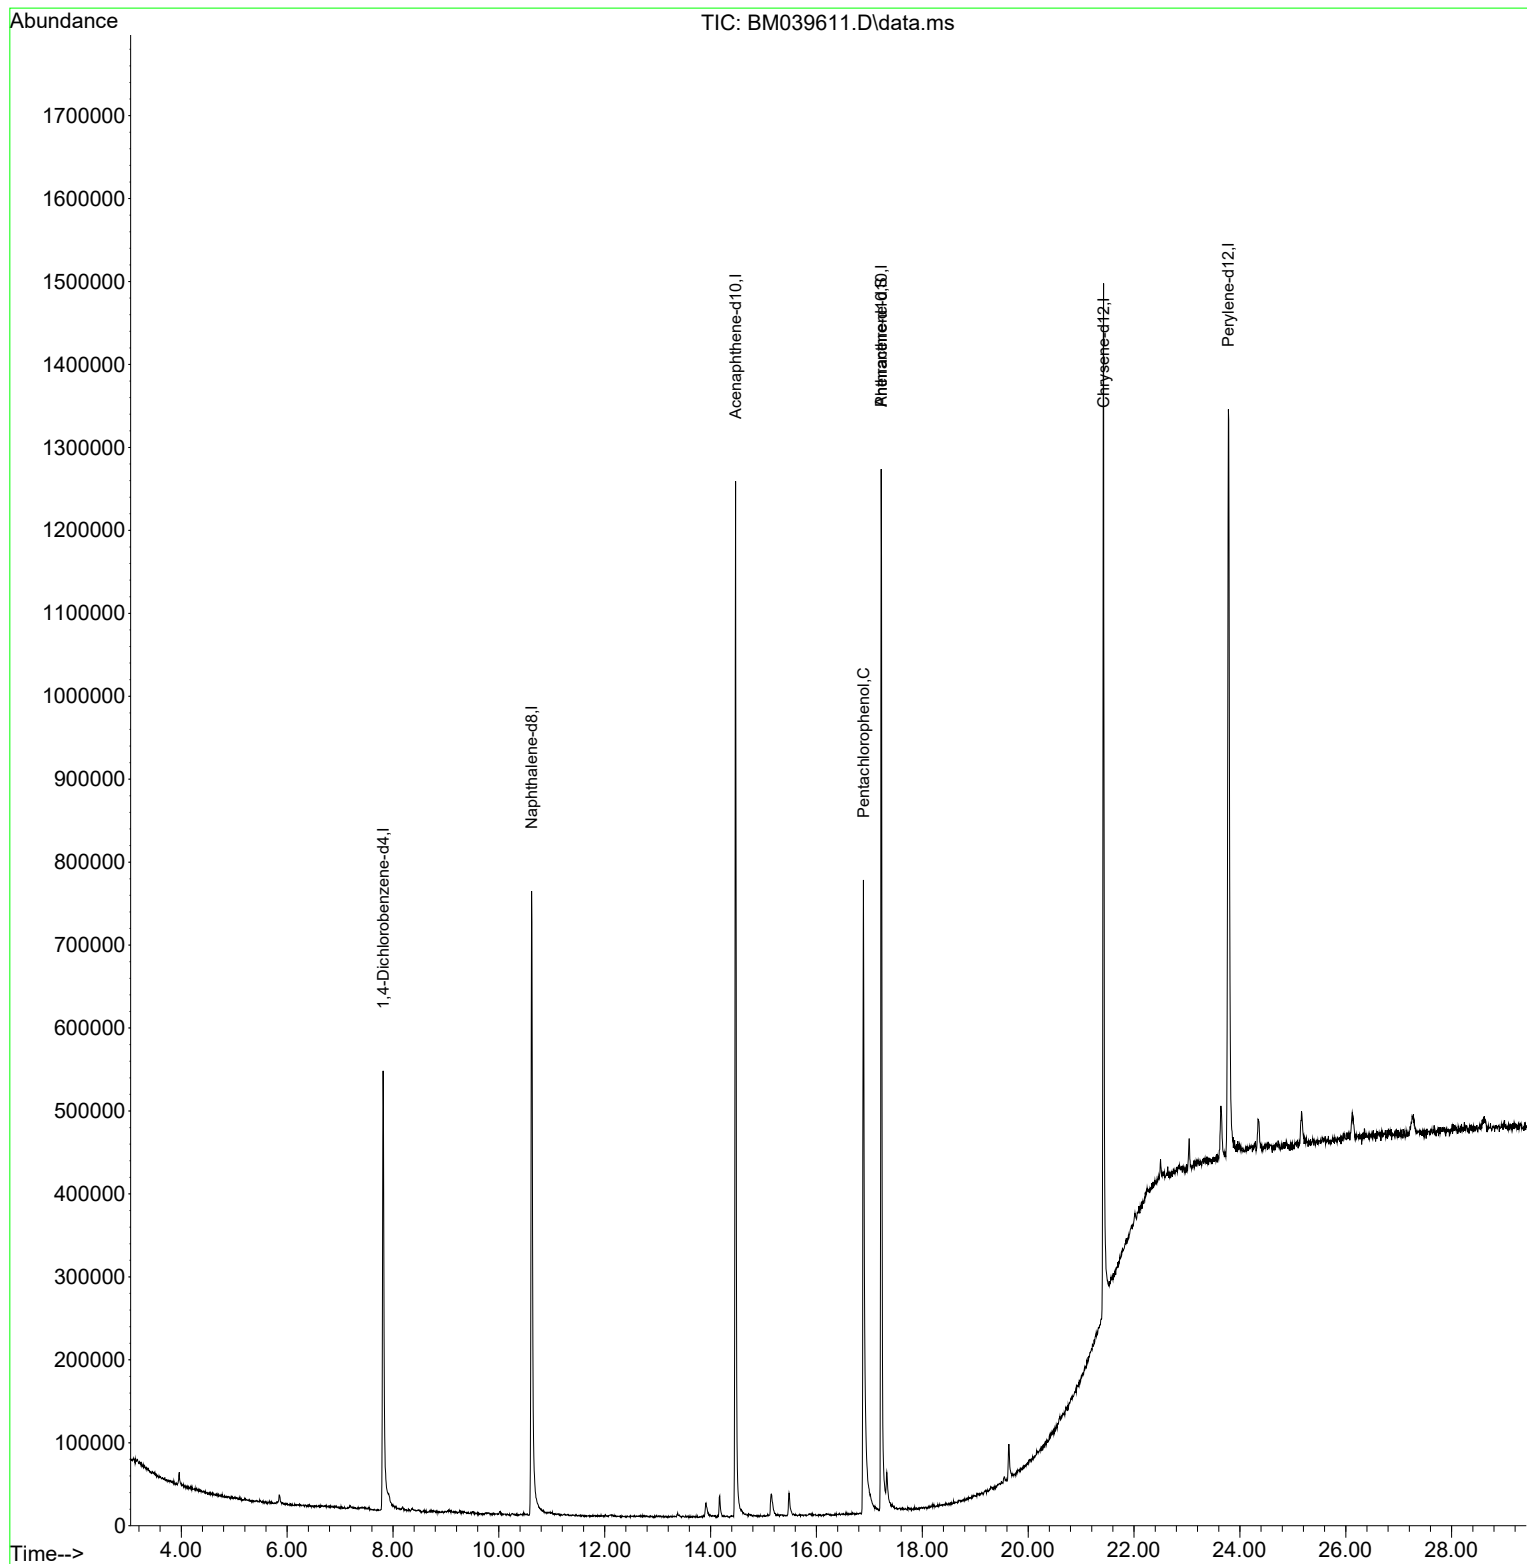

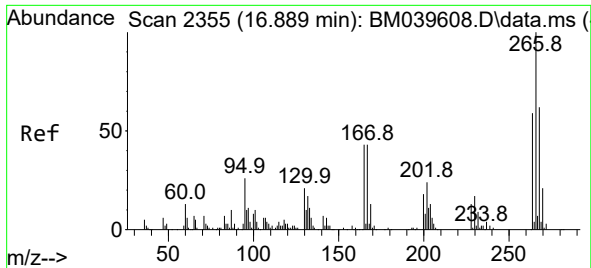

#71
 Pentachlorophenol
 Concen: 31.249 ng/ul
 RT: 16.889 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BM039611.D
 Acq: 24 Apr 2023 11:44

Instrument :
 BNA_M
 ClientSampleId :
 C0QG4DL2

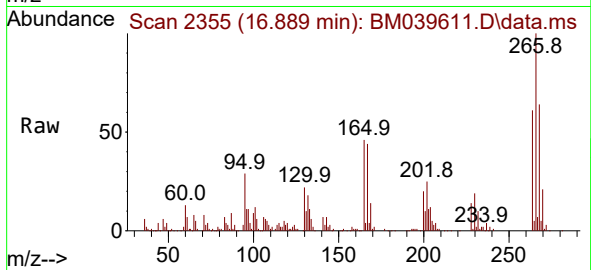

Tgt Ion:266 Resp: 185145
 Ion Ratio Lower Upper
 266 100
 264 60.5 50.2 75.4
 268 64.1 51.9 77.9

