




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039614.D
Acq On : 24 Apr 2023 13:32
Operator : CG/JU
Sample : PB152278BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK278

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/25/2023
Supervised By :Jagrut Upadhyay 04/25/2023

Quant Time: Apr 25 00:13:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 00:18:16 2023
Response via : Initial Calibration

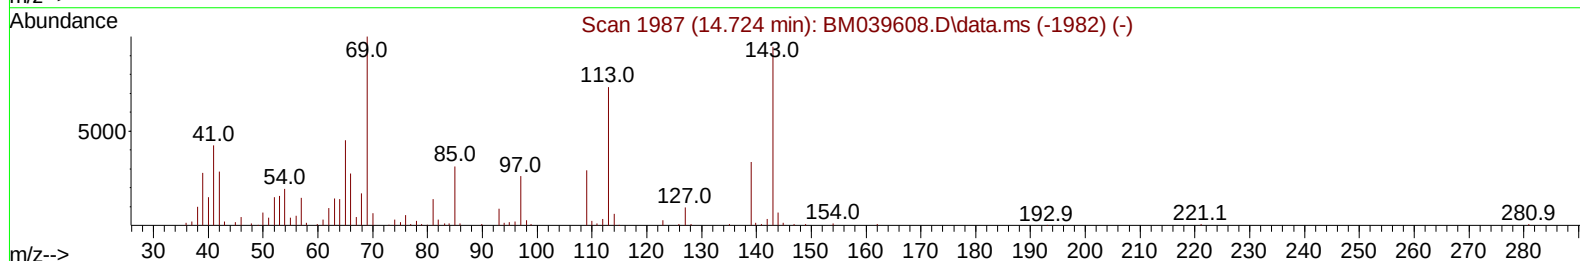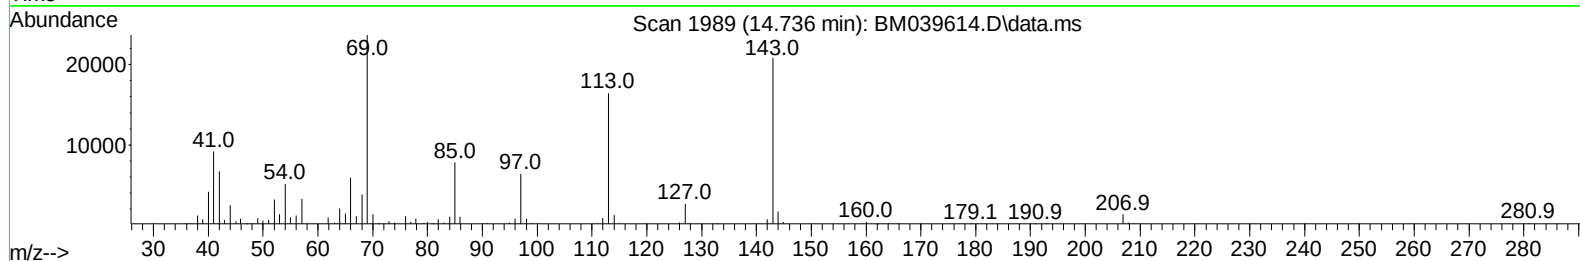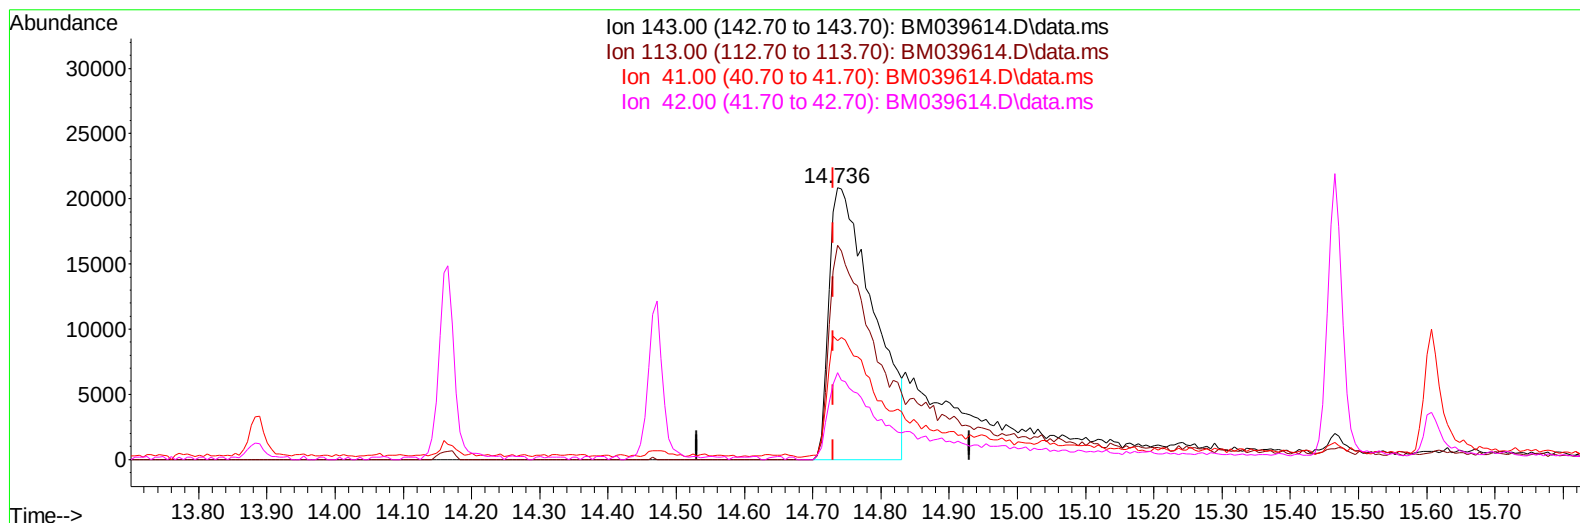

TIC: BM039614.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.736min (+ 0.006) 15.45 ng/ul

response 93758

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.20	78.92
41.00	39.90	43.86
42.00	26.60	32.05#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039614.D
Acq On : 24 Apr 2023 13:32
Operator : CG/JU
Sample : PB152278BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK278

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/25/2023
Supervised By :Jagrut Upadhyay 04/25/2023

Quant Time: Apr 25 00:13:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 00:18:16 2023
Response via : Initial Calibration

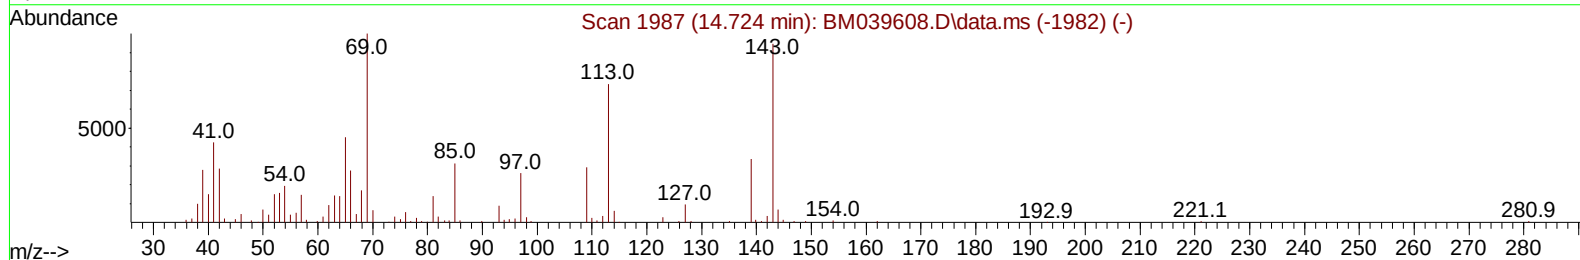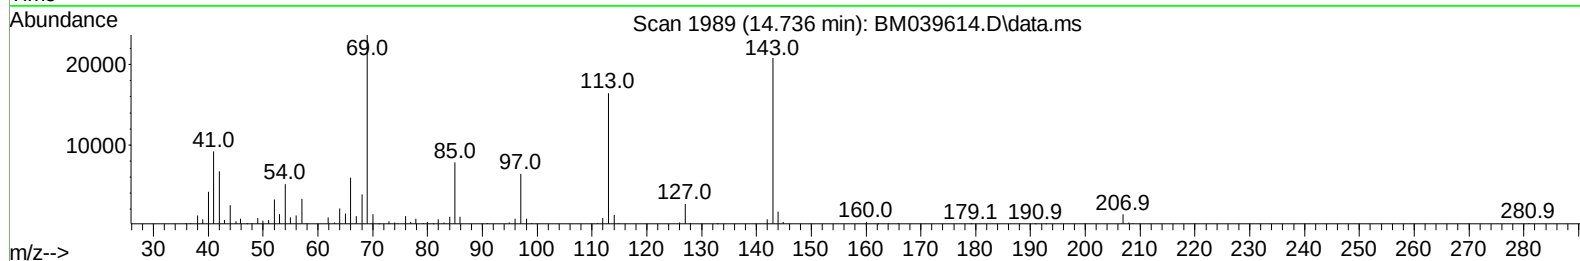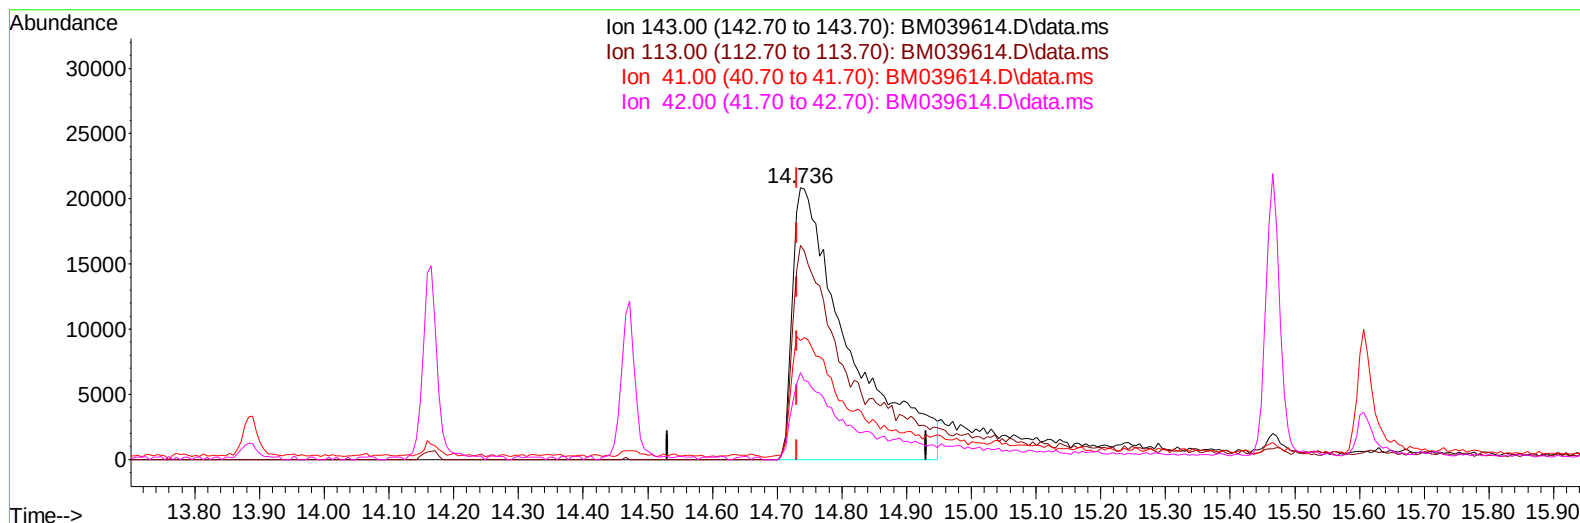

TIC: BM039614.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.736min (+ 0.006) 20.56 ng/ul m

response 124793

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	75.20	78.92
41.00	39.90	43.86
42.00	26.60	32.05#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
 Data File : BM039614.D
 Acq On : 24 Apr 2023 13:32
 Operator : CG/JU
 Sample : PB152278BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK278

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/25/2023
 Supervised By :Jagrut Upadhyay 04/25/2023

Quant Time: Apr 25 00:37:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Apr 23 00:18:16 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.813	152	193830	20.000	ng/ul	0.00
20) Naphthalene-d8	10.619	136	832788	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.471	164	497332	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.224	188	983276	20.000	ng/ul	0.00
79) Chrysene-d12	21.424	240	760689	20.000	ng/ul	0.00
88) Perylene-d12	23.788	264	823773	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.207	96	35028	6.937	ng/uL	0.00
4) Pyridine-d5	3.631	84	440102	31.018	ng/ul	0.00
7) Phenol-d5	6.995	99	548744	30.932	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.148	67	402860	34.357	ng/ul	0.00
11) 2-Chlorophenol-d4	7.343	132	467229	33.575	ng/ul	0.00
15) 4-Methylphenol-d8	8.542	113	446813	31.267	ng/ul	0.00
21) Nitrobenzene-d5	8.984	128	221758	33.098	ng/ul	0.00
24) 2-Nitrophenol-d4	9.707	143	254327	33.805	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.254	165	390102	30.135	ng/ul	0.00
31) 4-Chloroaniline-d4	10.772	131	560086	28.969	ng/ul	0.00
46) Dimethylphthalate-d6	13.883	166	1391797	34.700	ng/ul	0.00
49) Acenaphthylene-d8	14.166	160	1589113	35.267	ng/ul	0.00
54) 4-Nitrophenol-d4	14.736	143	124793m	20.558	ng/ul	0.00
60) Fluorene-d10	15.466	176	1151016	35.026	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.607	200	166788	25.525	ng/ul	0.00
73) Anthracene-d10	17.324	188	1741893	36.836	ng/ul	0.00
81) Pyrene-d10	19.624	212	1866131	36.918	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.630	264	1588988	35.728	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039614.D
Acq On : 24 Apr 2023 13:32
Operator : CG/JU
Sample : PB152278BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK278

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/25/2023
Supervised By :Jagrut Upadhyay 04/25/2023

Quant Time: Apr 25 00:37:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Apr 23 00:18:16 2023
Response via : Initial Calibration

