

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
 Data File : BM039611.D
 Acq On : 24 Apr 2023 11:44
 Operator : CG/JU
 Sample : 02462-01DL2 50X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0QG4DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs : 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039611.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.960	155	157	164	rVB	15712	19252	0.94%	0.149%
2	5.848	476	478	484	rVB4	9047	13104	0.64%	0.101%
3	7.548	765	767	769	rVB2	3934	2937	0.14%	0.023%
4	7.813	805	812	829	rBV	529075	1072825	52.47%	8.307%
5	8.178	872	874	878	rVB5	3902	5291	0.26%	0.041%
6	8.366	902	906	910	rBV6	2528	3245	0.16%	0.025%
7	9.101	1030	1031	1036	rBV5	2430	2549	0.12%	0.020%
8	9.236	1050	1054	1056	rBV5	1547	2303	0.11%	0.018%
9	9.348	1070	1073	1076	rBV5	1889	2188	0.11%	0.017%
10	9.748	1138	1141	1142	rBV3	1949	2061	0.10%	0.016%
11	9.801	1148	1150	1156	rVB7	2623	5152	0.25%	0.040%
12	10.025	1183	1188	1194	rVB9	4296	8026	0.39%	0.062%
13	10.254	1220	1227	1233	rBV9	3238	9726	0.48%	0.075%
14	10.472	1261	1264	1265	rVV3	3582	2944	0.14%	0.023%
15	10.489	1265	1267	1271	rVV5	1887	2991	0.15%	0.023%
16	10.536	1271	1275	1277	rVB5	1893	2279	0.11%	0.018%
17	10.619	1282	1289	1317	rBV	752285	1576324	77.10%	12.206%
18	11.583	1450	1453	1457	rVB5	1652	2393	0.12%	0.019%
19	12.424	1595	1596	1602	rBV6	1418	2152	0.11%	0.017%
20	12.489	1606	1607	1611	rBV4	2122	2204	0.11%	0.017%
21	13.377	1754	1758	1760	rBV5	4617	5560	0.27%	0.043%
22	13.407	1762	1763	1770	rVB7	3109	4340	0.21%	0.034%
23	13.465	1770	1773	1774	rBV3	1958	2107	0.10%	0.016%
24	13.571	1789	1791	1794	rVB4	2294	2861	0.14%	0.022%
25	13.913	1843	1849	1856	rBV	16987	40824	2.00%	0.316%
26	13.989	1861	1862	1868	rVB6	2282	2102	0.10%	0.016%
27	14.171	1889	1893	1901	rVB2	24867	44479	2.18%	0.344%
28	14.471	1938	1944	1959	rBV	1248459	1993438	97.50%	15.435%
29	14.724	1984	1987	1989	rBV4	2408	2832	0.14%	0.022%
30	15.148	2053	2059	2070	rBV5	25558	73607	3.60%	0.570%
31	15.318	2085	2088	2089	rBV3	1781	2073	0.10%	0.016%
32	15.483	2109	2116	2127	rBV	27686	63730	3.12%	0.493%
33	15.565	2127	2130	2135	rVB6	2011	2862	0.14%	0.022%
34	15.654	2143	2145	2150	rBV5	1400	2574	0.13%	0.020%
35	15.877	2181	2183	2187	rVB4	2180	2768	0.14%	0.021%
36	16.048	2210	2212	2215	rBV4	2242	2495	0.12%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039611.D
Acq On : 24 Apr 2023 11:44
Operator : CG/JU
Sample : 02462-01DL2 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0QG4DL2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Title : SVOA CALIBRATION

37	16.183	2231	2235	2236	rBV4	1947	2367	0.12%	0.018%
38	16.259	2246	2248	2251	rVB4	2071	2079	0.10%	0.016%
39	16.889	2348	2355	2387	rBV	764507	1746199	85.41%	13.521%
40	17.224	2406	2412	2426	rBV	1255150	2044476	100.00%	15.831%
41	17.330	2426	2430	2440	rVB2	37547	83745	4.10%	0.648%
42	17.842	2515	2517	2518	rBV2	2715	2332	0.11%	0.018%
43	17.965	2535	2538	2539	rBV2	2024	2211	0.11%	0.017%
44	19.636	2817	2822	2831	rBV2	44390	94413	4.62%	0.731%
45	21.424	3121	3126	3142	rBV	1236561	2002938	97.97%	15.509%
46	23.782	3521	3527	3541	rBV2	880723	1945353	95.15%	15.063%




Sum of corrected areas: 12914711

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039611.D
Acq On : 24 Apr 2023 11:44
Operator : CG/JU
Sample : 02462-01DL2 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0QG4DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

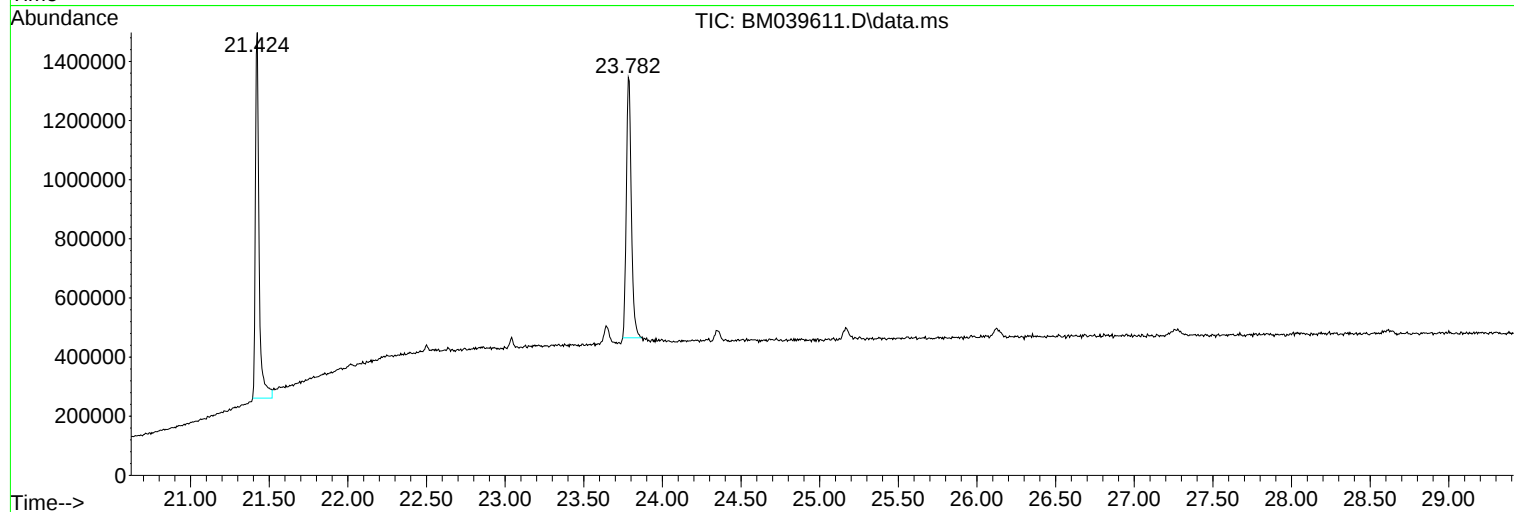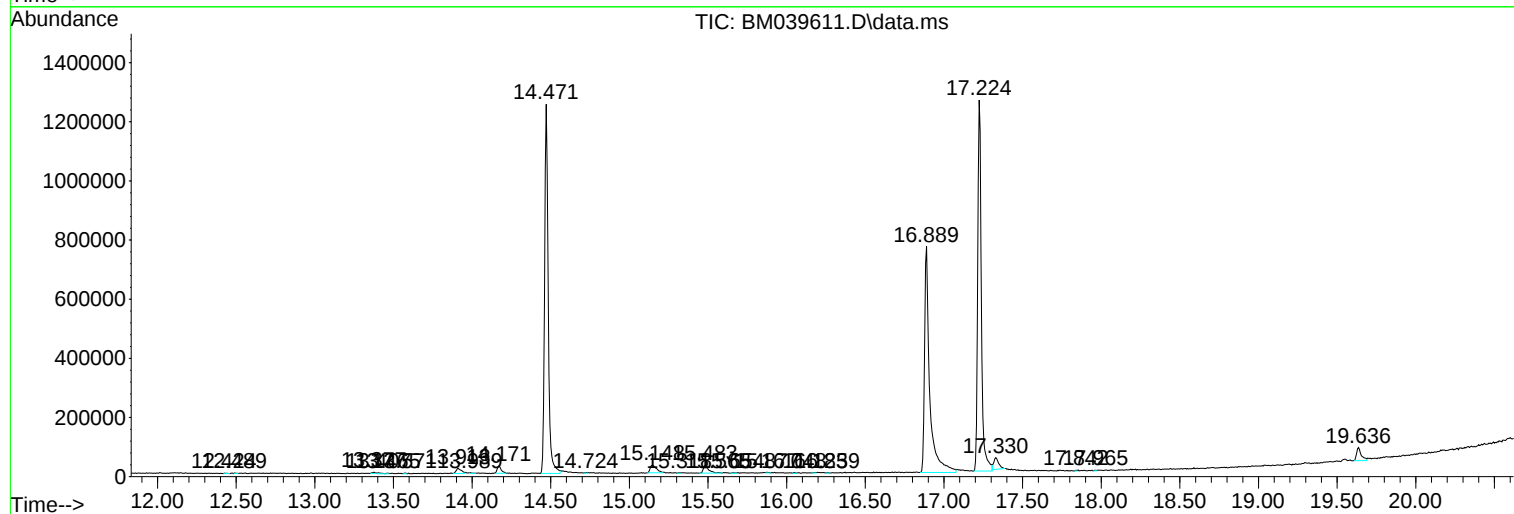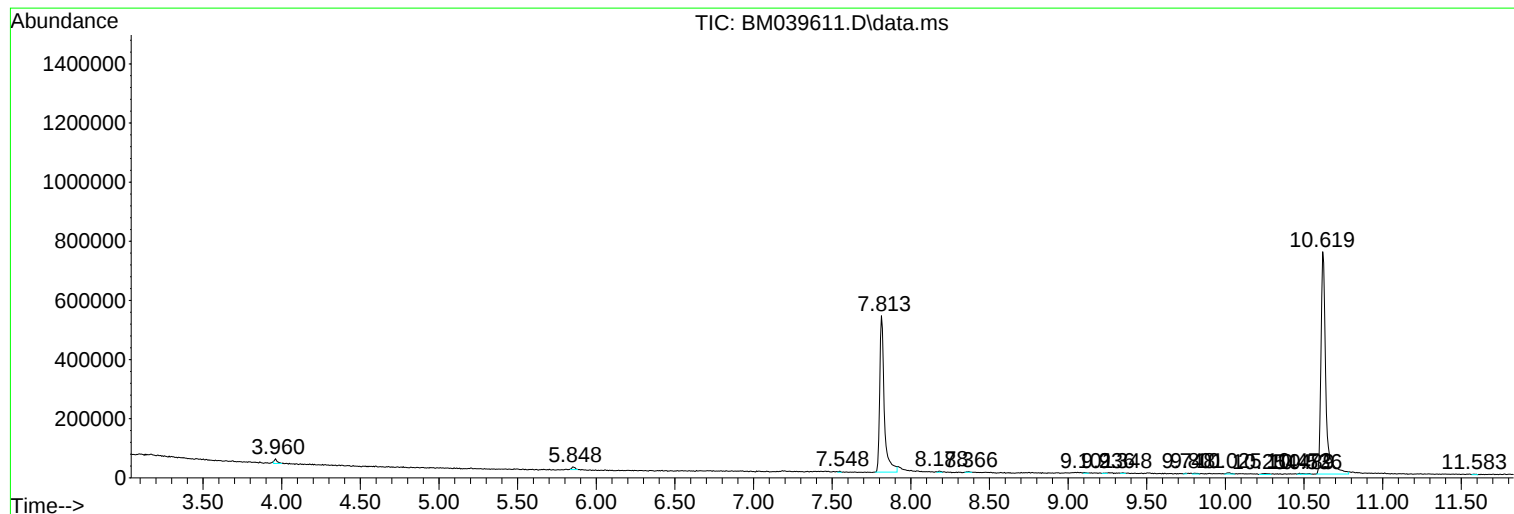

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039611.D
Acq On : 24 Apr 2023 11:44
Operator : CG/JU
Sample : 02462-01DL2 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0QG4DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039611.D
Acq On : 24 Apr 2023 11:44
Operator : CG/JU
Sample : 02462-01DL2 50X
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0QG4DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc