

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
 Data File : BM039614.D
 Acq On : 24 Apr 2023 13:32
 Operator : CG/JU
 Sample : PB152278BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK278

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039614.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.207	25	29	37	rVB	77550	101840	2.05%	0.187%
2	3.631	98	101	126	rBV	782546	1269723	25.55%	2.329%
3	3.960	154	157	163	rVB2	15737	24641	0.50%	0.045%
4	6.995	667	673	693	rBV	794795	1578863	31.78%	2.896%
5	7.148	693	699	719	rVB	820742	1406048	28.30%	2.579%
6	7.343	726	732	755	rBV	944308	1701962	34.25%	3.122%
7	7.813	805	812	825	rBV	683687	1197622	24.10%	2.197%
8	8.542	930	936	962	rBV	1018531	2013475	40.52%	3.693%
9	8.984	1004	1011	1025	rBV	900156	1626493	32.73%	2.983%
10	9.707	1127	1134	1150	rBV	752064	1408624	28.35%	2.584%
11	10.254	1221	1227	1252	rBV	819770	1895652	38.15%	3.477%
12	10.619	1282	1289	1303	rBV	999240	1729901	34.81%	3.173%
13	10.772	1308	1315	1338	rBV	874027	1926291	38.77%	3.533%
14	12.242	1560	1565	1567	rBV6	9719	15504	0.31%	0.028%
15	13.372	1751	1757	1764	rVB5	7930	15528	0.31%	0.028%
16	13.883	1838	1844	1860	rBV	1986825	3094847	62.28%	5.677%
17	14.166	1884	1892	1910	rBV	2380087	3755445	75.58%	6.888%
18	14.471	1936	1944	1963	rBV	1522398	2272329	45.73%	4.168%
19	14.736	1983	1989	2012	rBV4	145163	749627	15.09%	1.375%
20	15.466	2107	2113	2131	rBV	2951739	4402909	88.61%	8.076%
21	15.607	2131	2137	2152	rBV	689045	1233890	24.83%	2.263%
22	16.901	2354	2357	2361	rVB6	4196	5112	0.10%	0.009%
23	17.012	2370	2376	2379	rBV7	3418	7969	0.16%	0.015%
24	17.224	2405	2412	2423	rBV	1730052	2452824	49.36%	4.499%
25	17.324	2423	2429	2451	rVB	3022377	4564277	91.86%	8.372%
26	19.189	2742	2746	2753	rBV3	34396	52166	1.05%	0.096%
27	19.265	2755	2759	2764	rBV	25107	40600	0.82%	0.074%
28	19.624	2814	2820	2841	rBV	3436239	4968864	100.00%	9.114%
29	21.424	3121	3126	3139	rBV	1414401	2230568	44.89%	4.091%
30	23.630	3494	3501	3517	rBV2	2142347	4578363	92.14%	8.398%
31	23.788	3521	3528	3540	rVB2	1003010	2197692	44.23%	4.031%




Sum of corrected areas: 54519649

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039614.D
Acq On : 24 Apr 2023 13:32
Operator : CG/JU
Sample : PB152278BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK278

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

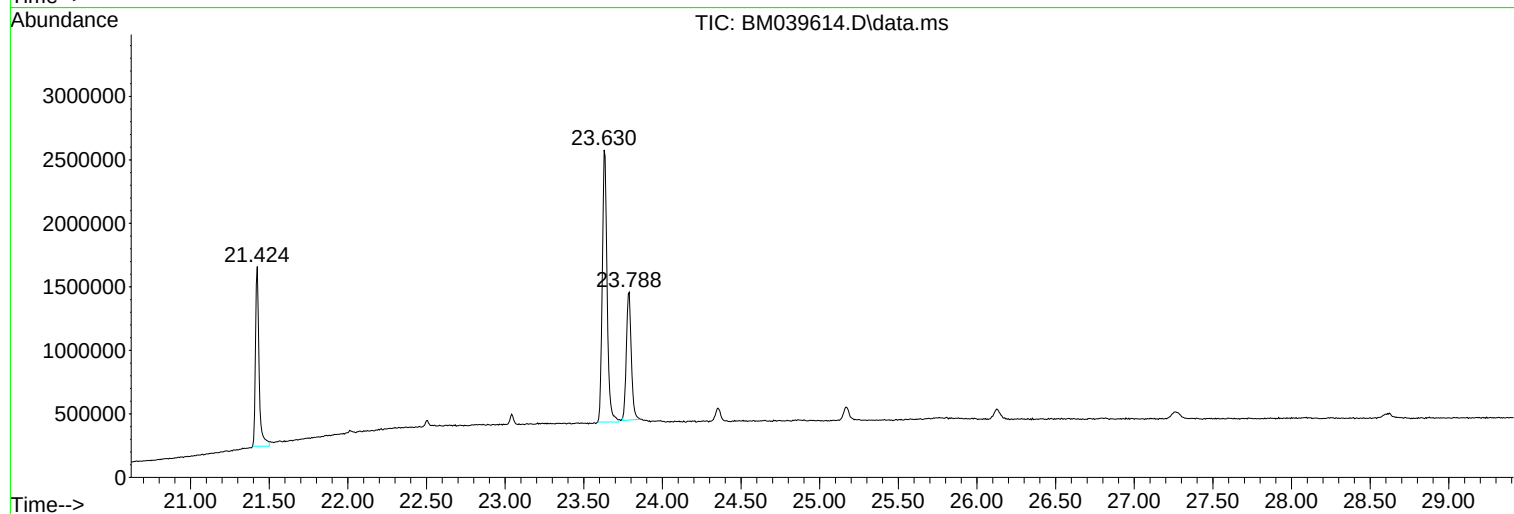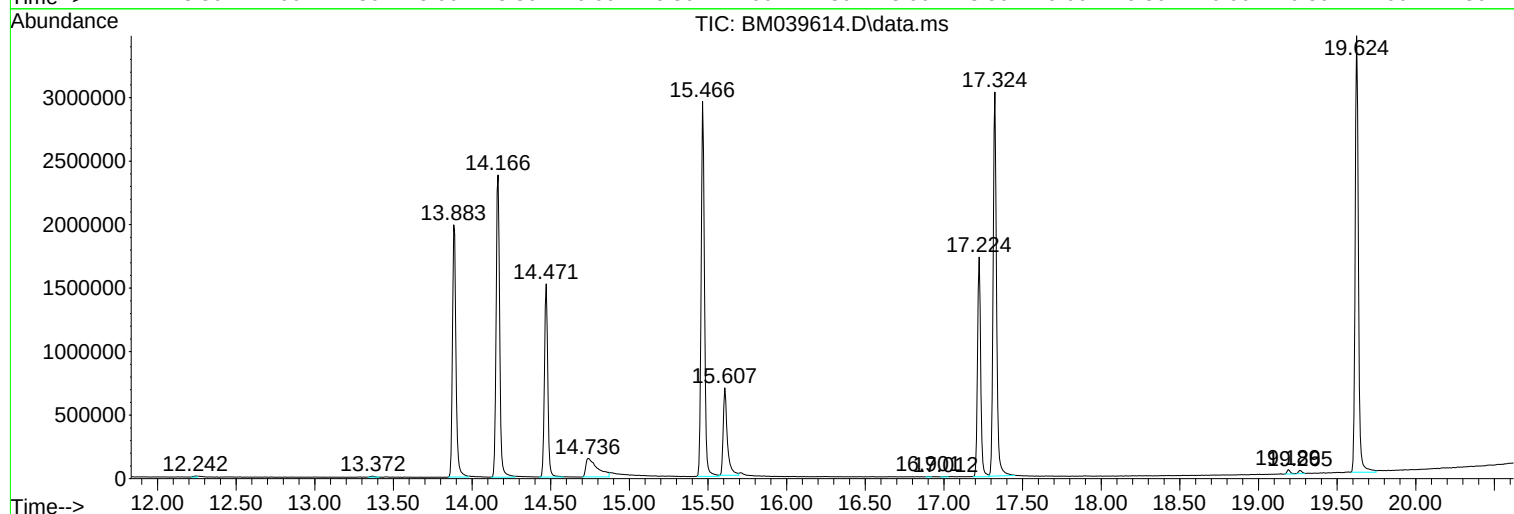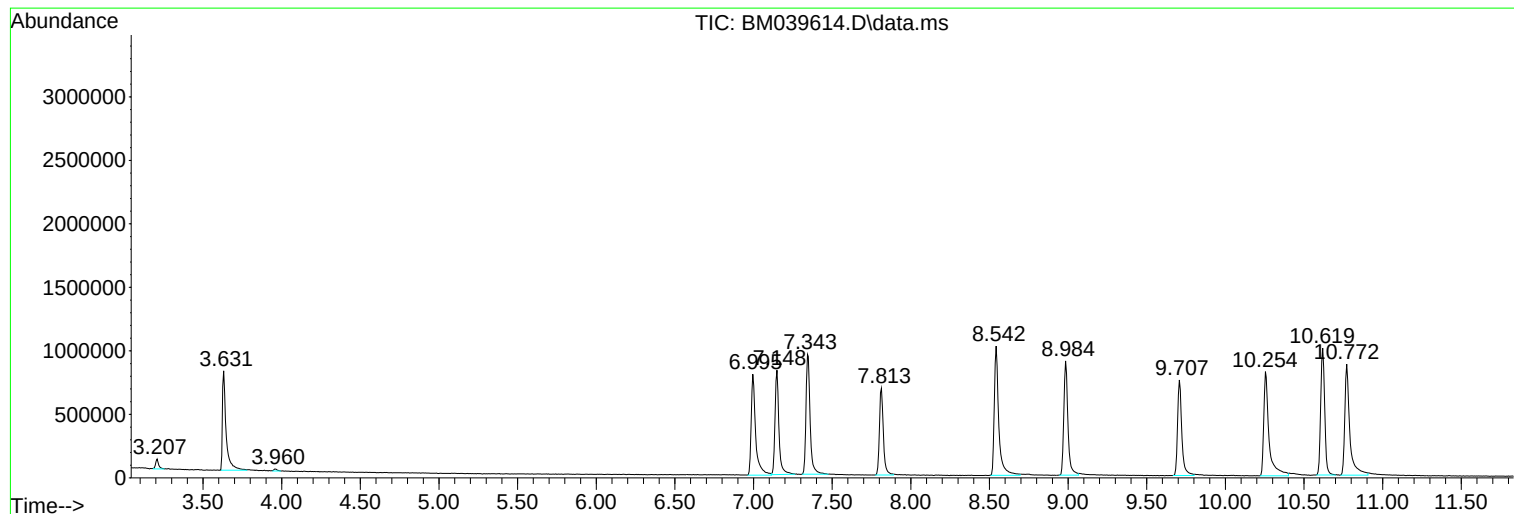

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039614.D
Acq On : 24 Apr 2023 13:32
Operator : CG/JU
Sample : PB152278BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK278

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039614.D
Acq On : 24 Apr 2023 13:32
Operator : CG/JU
Sample : PB152278BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK278

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc