

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
 Data File : BM039617.D
 Acq On : 24 Apr 2023 16:20
 Operator : CG/JU
 Sample : PB152350BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK350

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.208	25	29	37	rVB	68561	93760	1.70%	0.165%
2	3.631	98	101	127	rBV	633761	1080793	19.61%	1.907%
3	6.996	667	673	691	rBV	713299	1432036	25.98%	2.527%
4	7.148	693	699	719	rVB	726047	1289842	23.40%	2.276%
5	7.343	726	732	755	rBV	890926	1570249	28.49%	2.771%
6	7.807	805	811	825	rBV	712626	1266536	22.98%	2.235%
7	8.542	928	936	958	rBV	909846	1876092	34.04%	3.310%
8	8.984	1003	1011	1026	rBV	828745	1533217	27.82%	2.705%
9	9.707	1126	1134	1152	rBV	699899	1332356	24.18%	2.351%
10	10.254	1221	1227	1255	rBV	721792	1776857	32.24%	3.135%
11	10.619	1280	1289	1302	rBV	1070735	1879851	34.11%	3.317%
12	10.772	1308	1315	1348	rBV	698737	1686993	30.61%	2.977%
13	12.248	1558	1566	1571	rBV7	8256	23672	0.43%	0.042%
14	13.366	1752	1756	1759	rBV5	5192	8153	0.15%	0.014%
15	13.883	1838	1844	1869	rBV	2022435	3126194	56.72%	5.516%
16	14.166	1885	1892	1911	rBV	2351402	3646993	66.17%	6.435%
17	14.472	1937	1944	1962	rBV	1677617	2555132	46.36%	4.509%
18	14.736	1982	1989	2012	rBV2	152620	791876	14.37%	1.397%
19	15.466	2106	2113	2129	rBV	2973314	4405186	79.93%	7.773%
20	15.607	2131	2137	2151	rBV	739539	1310065	23.77%	2.312%
21	17.224	2405	2412	2422	rBV	1986663	2961381	53.73%	5.225%
22	17.324	2422	2429	2451	rVB	3198368	4812780	87.33%	8.492%
23	19.189	2742	2746	2753	rBV2	35693	51926	0.94%	0.092%
24	19.265	2755	2759	2766	rVV	28880	49284	0.89%	0.087%
25	19.624	2814	2820	2839	rBV	3903124	5511140	100.00%	9.725%
26	21.424	3120	3126	3140	rBV	1939252	3042804	55.21%	5.369%
27	23.630	3494	3501	3518	rBV2	2315029	4804115	87.17%	8.477%
28	23.783	3521	3527	3544	rVB2	1248120	2752840	49.95%	4.857%




Sum of corrected areas: 56672123

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039617.D
Acq On : 24 Apr 2023 16:20
Operator : CG/JU
Sample : PB152350BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK350

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

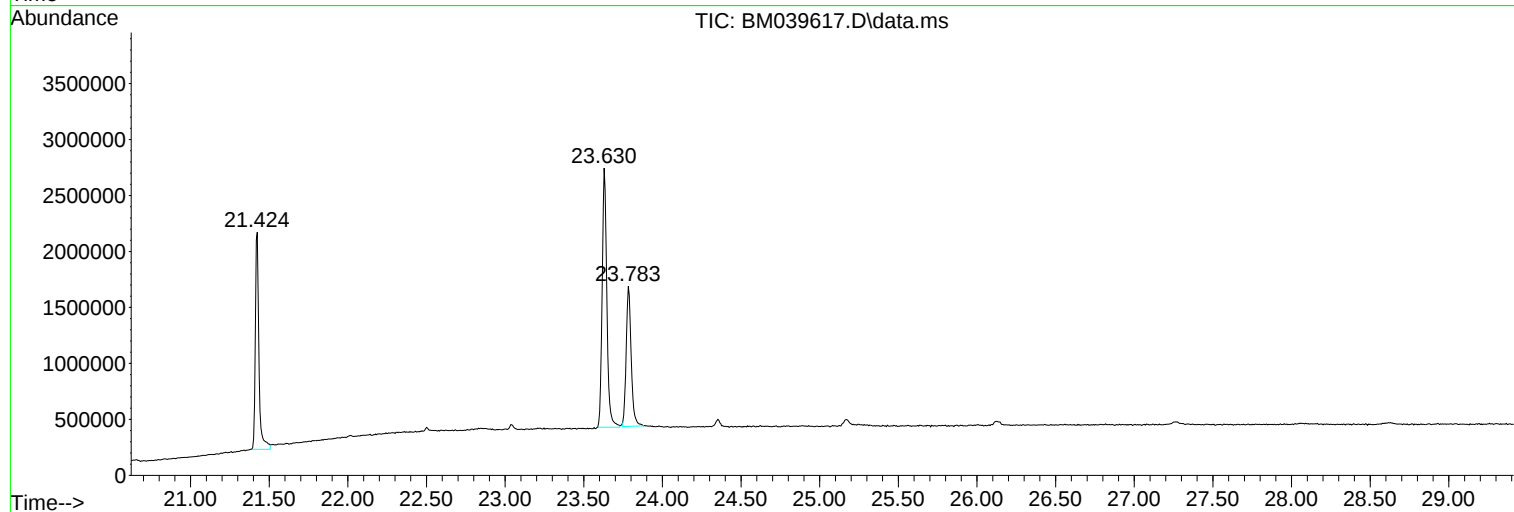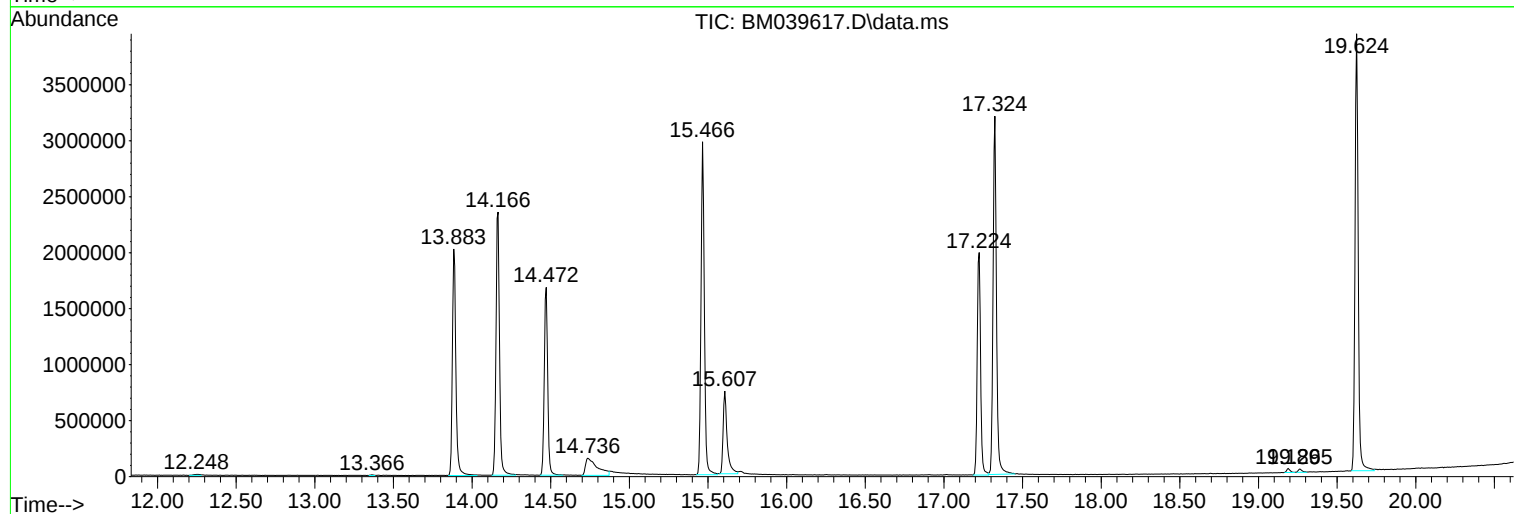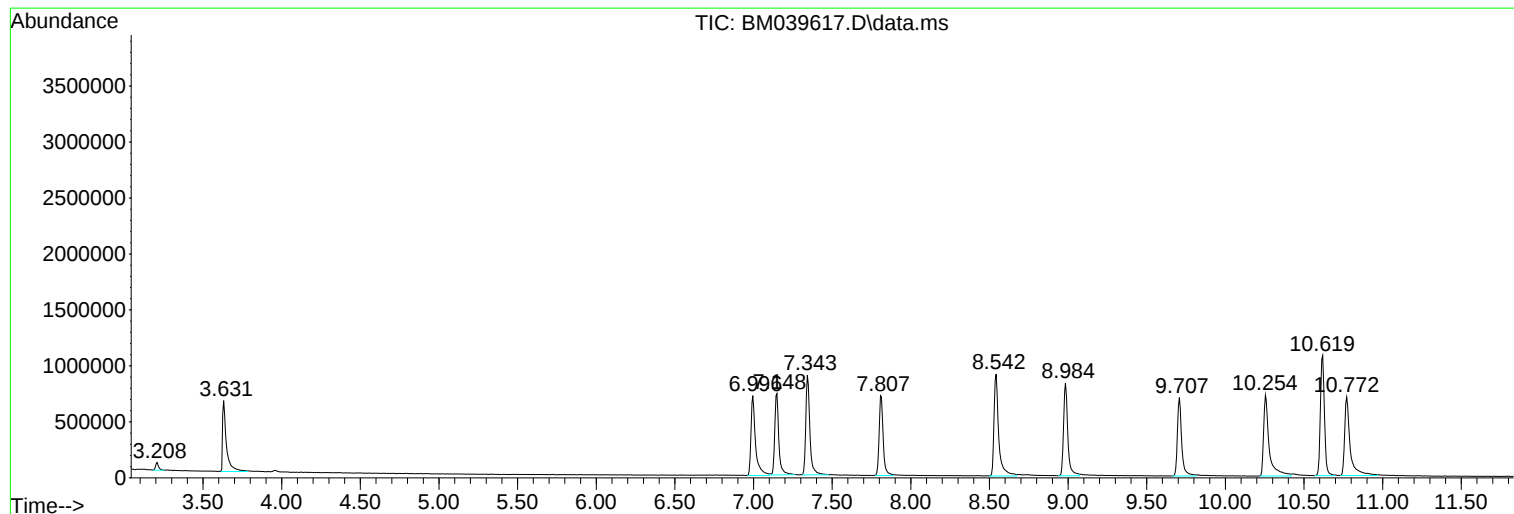

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039617.D
Acq On : 24 Apr 2023 16:20
Operator : CG/JU
Sample : PB152350BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK350

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039617.D
Acq On : 24 Apr 2023 16:20
Operator : CG/JU
Sample : PB152350BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK350

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------