

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
 Data File : BM039630.D
 Acq On : 25 Apr 2023 00:08
 Operator : CG/JU
 Sample : PB152352BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK352

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM039630.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.208	25	29	36	rVB	61291	89683	1.42%	0.145%
2	3.631	98	101	127	rBV	609887	1130058	17.89%	1.828%
3	3.955	154	156	161	rVB3	14055	18012	0.29%	0.029%
4	6.996	666	673	692	rBV	709508	1433084	22.69%	2.319%
5	7.143	692	698	725	rVB	710253	1270197	20.11%	2.055%
6	7.343	726	732	748	rBV	878393	1516368	24.00%	2.453%
7	7.807	805	811	831	rBV	695360	1217063	19.27%	1.969%
8	8.537	929	935	963	rBV	913289	1870120	29.60%	3.026%
9	8.984	1002	1011	1033	rBV	823735	1548502	24.51%	2.505%
10	9.707	1126	1134	1157	rBV	689115	1349117	21.36%	2.183%
11	10.254	1220	1227	1255	rBV	757341	1762610	27.90%	2.852%
12	10.619	1281	1289	1303	rBV	1041176	1837493	29.09%	2.973%
13	10.772	1308	1315	1334	rBV	720280	1648659	26.10%	2.667%
14	12.236	1557	1564	1573	rBV7	8472	26028	0.41%	0.042%
15	13.366	1752	1756	1762	rBV6	7771	12139	0.19%	0.020%
16	13.883	1838	1844	1863	rBV	2213025	3288442	52.06%	5.320%
17	14.160	1884	1891	1909	rBV	2513944	3889379	61.57%	6.293%
18	14.466	1936	1943	1961	rBV	1761835	2729484	43.21%	4.416%
19	14.583	1961	1963	1970	rVB6	4105	7508	0.12%	0.012%
20	14.730	1981	1988	2019	rBV2	195922	1042055	16.50%	1.686%
21	15.466	2106	2113	2131	rBV	3146300	4713625	74.62%	7.626%
22	15.607	2131	2137	2152	rVV	822676	1476165	23.37%	2.388%
23	15.707	2152	2154	2161	rVB4	22305	33604	0.53%	0.054%
24	17.013	2371	2376	2378	rBV4	4779	6542	0.10%	0.011%
25	17.224	2405	2412	2422	rBV	2101226	3168967	50.17%	5.127%
26	17.318	2422	2428	2450	rVB	3393289	5133718	81.27%	8.306%
27	19.189	2742	2746	2752	rBV3	39555	56395	0.89%	0.091%
28	19.259	2754	2758	2765	rVV	30746	51645	0.82%	0.084%
29	19.618	2813	2819	2831	rBV	4088570	6021831	95.33%	9.743%
30	21.418	3120	3125	3140	rBV	2326340	3411176	54.00%	5.519%
31	23.036	3397	3400	3408	rVB2	135498	203370	3.22%	0.329%
32	23.624	3493	3500	3517	rBV	3150127	6316934	100.00%	10.220%
33	23.777	3519	3526	3542	rVB2	1632863	3527747	55.85%	5.708%




Sum of corrected areas: 61807720

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039630.D
Acq On : 25 Apr 2023 00:08
Operator : CG/JU
Sample : PB152352BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK352

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

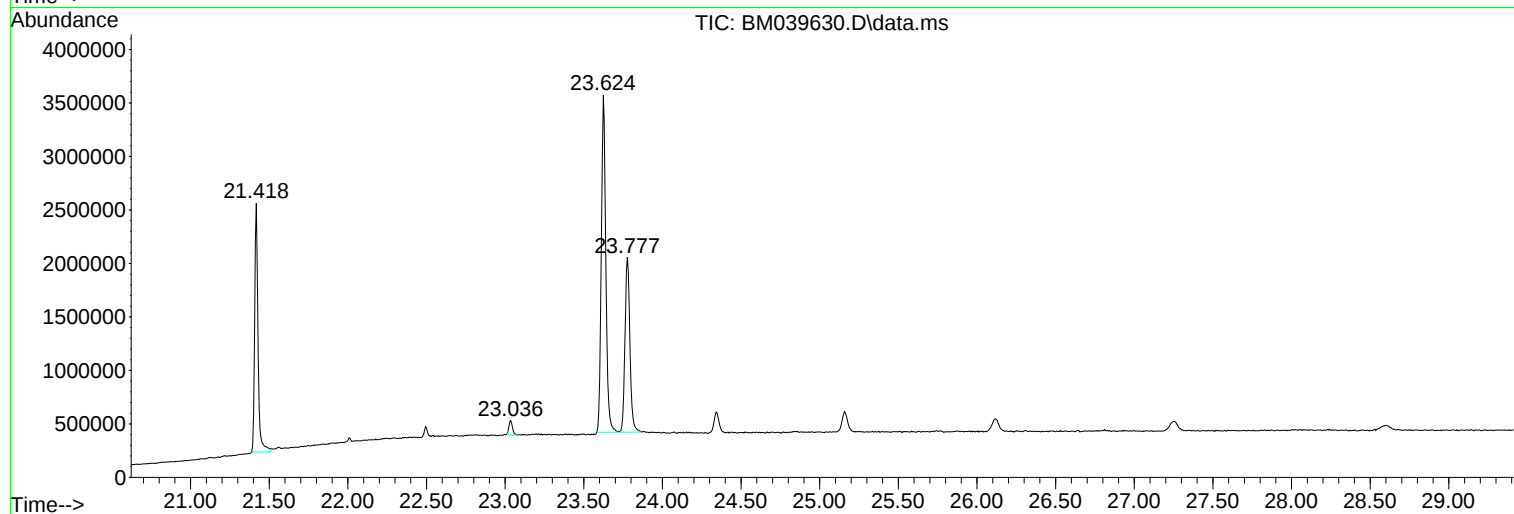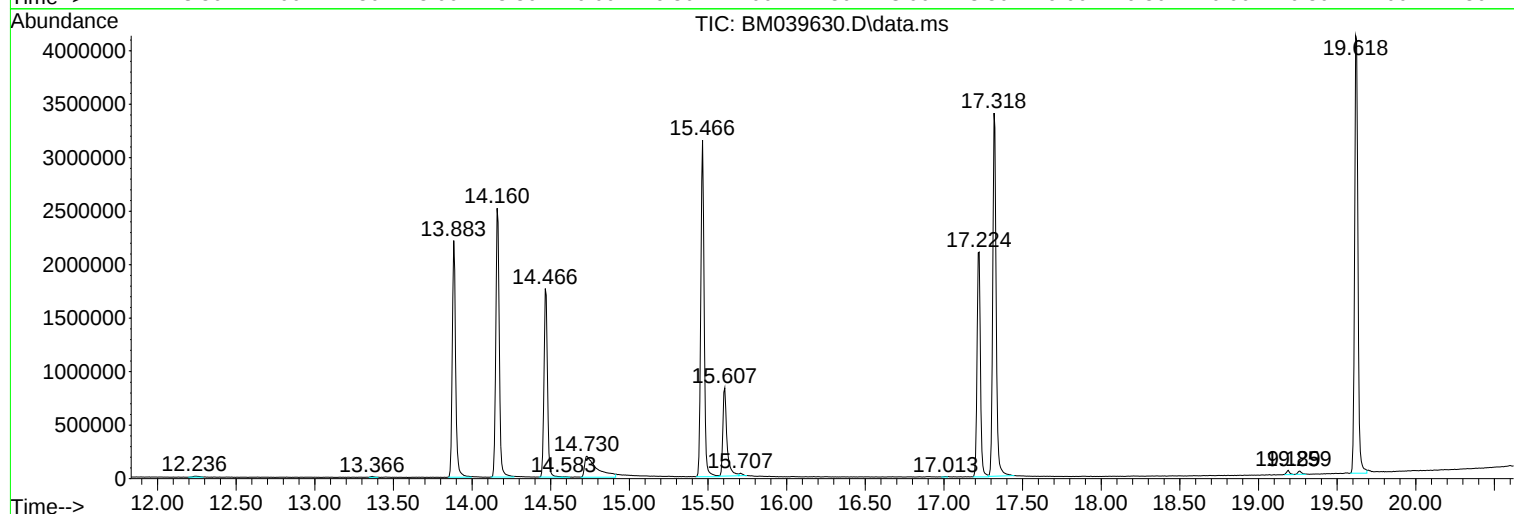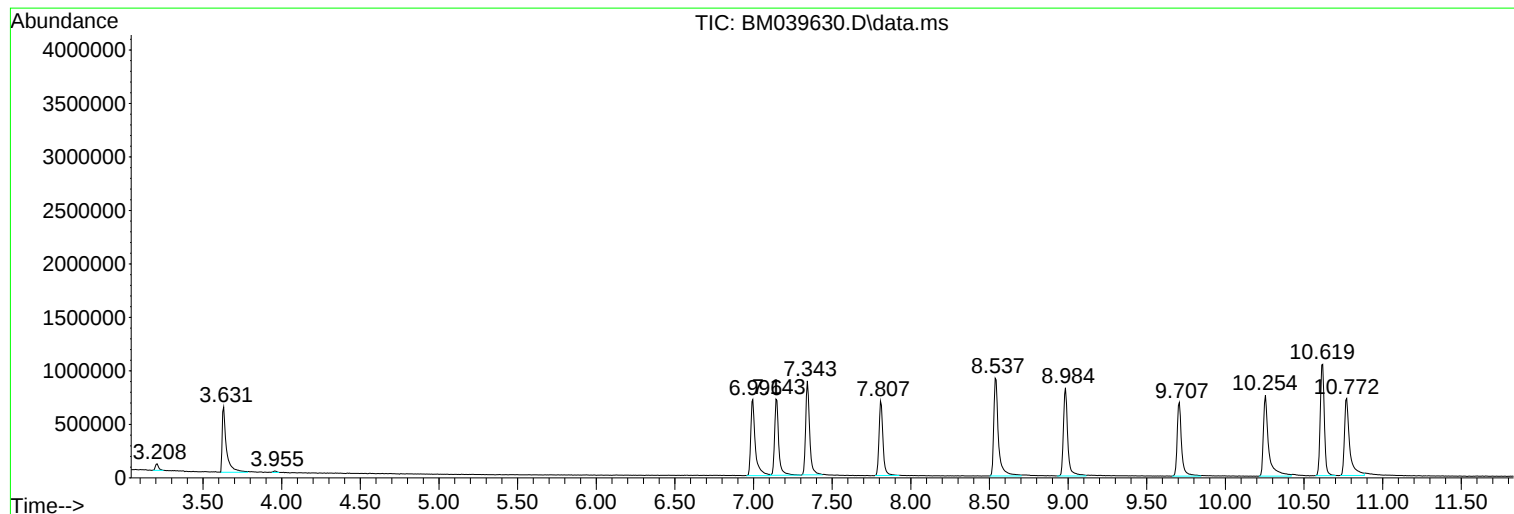

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039630.D
Acq On : 25 Apr 2023 00:08
Operator : CG/JU
Sample : PB152352BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK352

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042423\
Data File : BM039630.D
Acq On : 25 Apr 2023 00:08
Operator : CG/JU
Sample : PB152352BL
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK352

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM041823.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc