
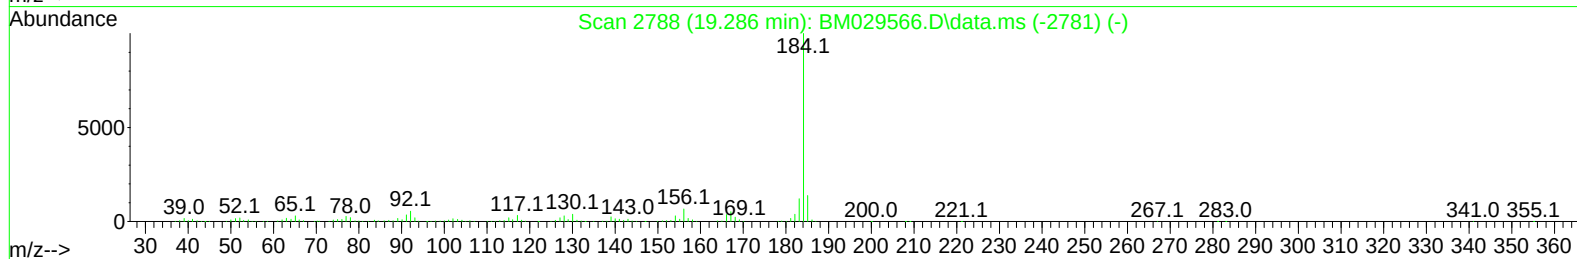
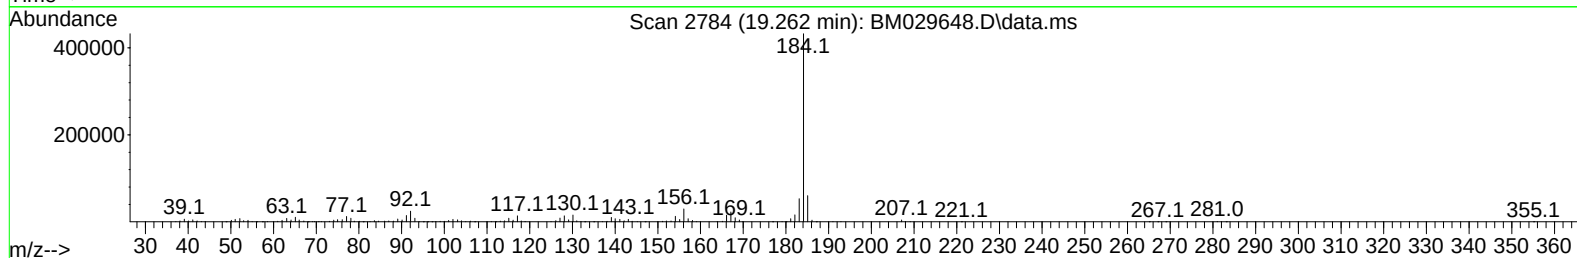


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042621\
 Data File : BM029648.D
 Acq On : 26 Apr 2021 13:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 14:29:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 22 15:55:11 2021
 Response via : Initial Calibration

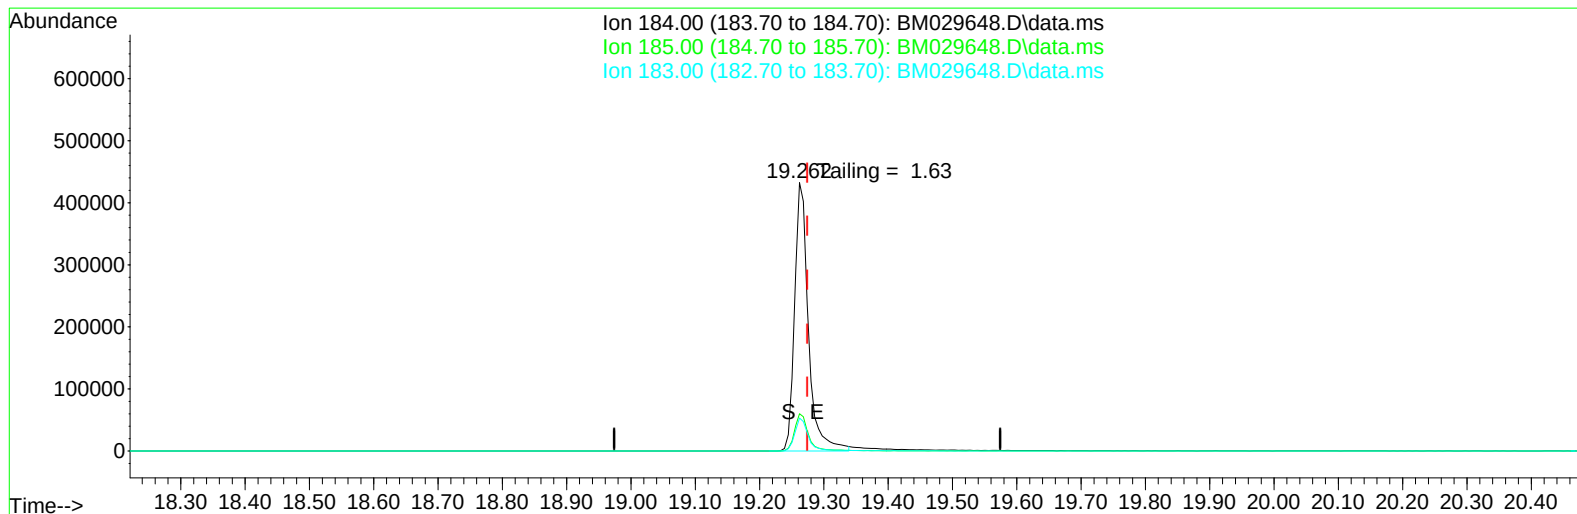

TIC: BM029648.D\data.ms

(77) Benzidine




19.262min (-0.012) 596763.26 ng

response 669648

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.92
183.00	12.30	12.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042621\
Data File : BM029648.D
Acq On : 26 Apr 2021 13:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 26 14:29:24 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 22 15:55:11 2021
Response via : Initial Calibration

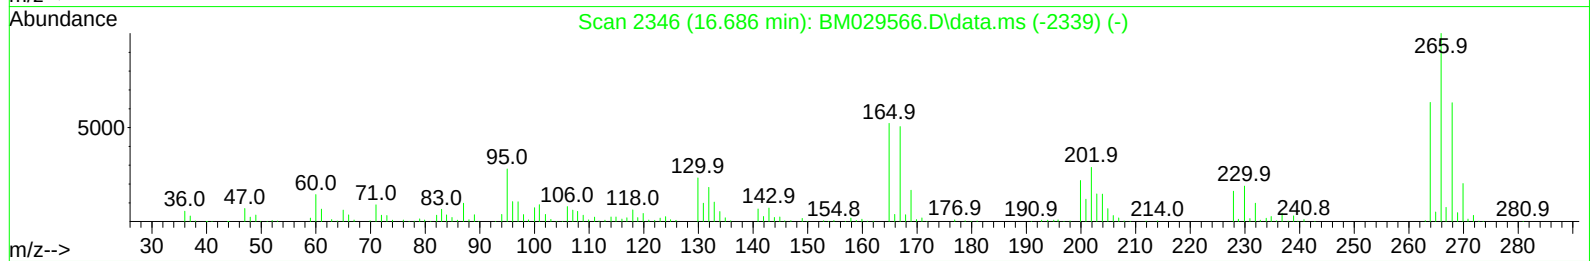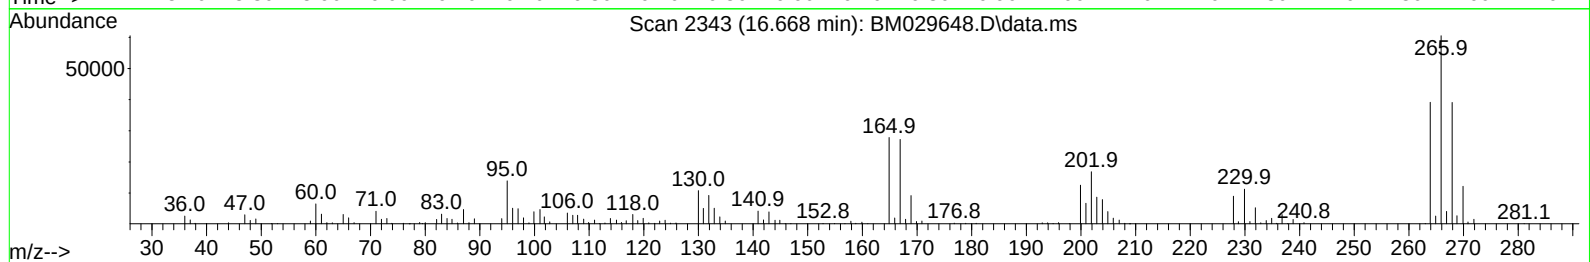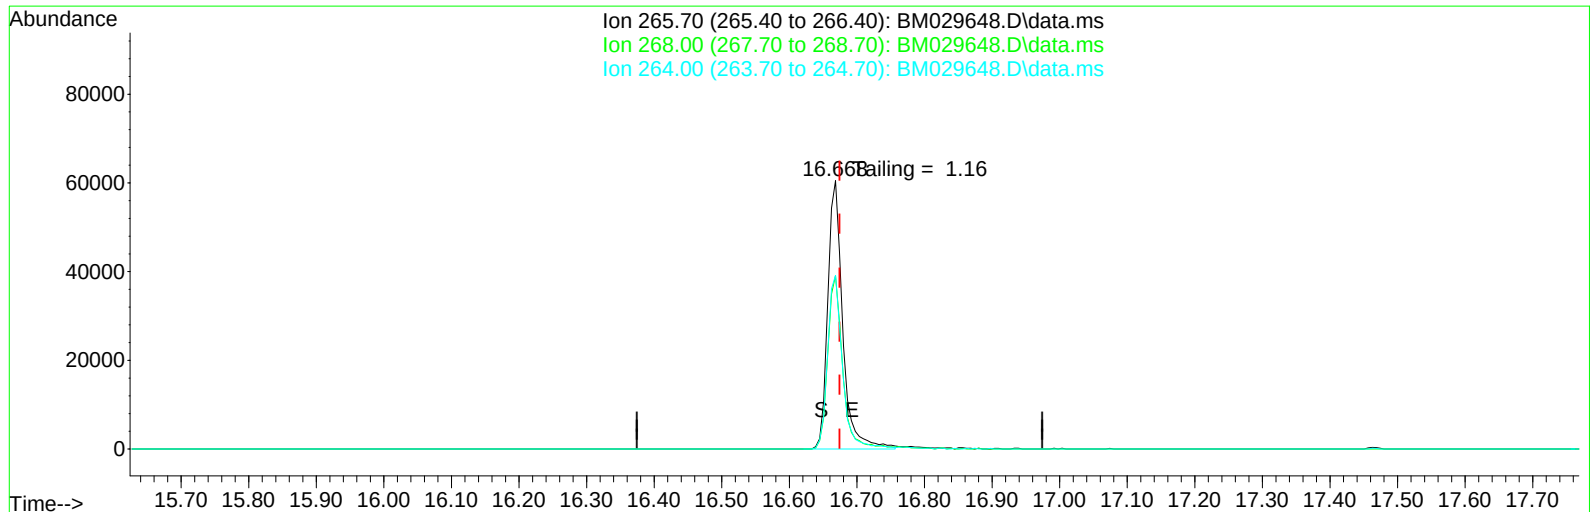

TIC: BM029648.D\data.ms

(70) Pentachlorophenol (C)

16.668min (-0.006) 0.00 ng

response 93548

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.64
264.00	64.90	64.69
0.00	0.00	0.00