


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042621\
 Data File : BM029648.D
 Acq On : 26 Apr 2021 13:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 26 15:01:01 2021

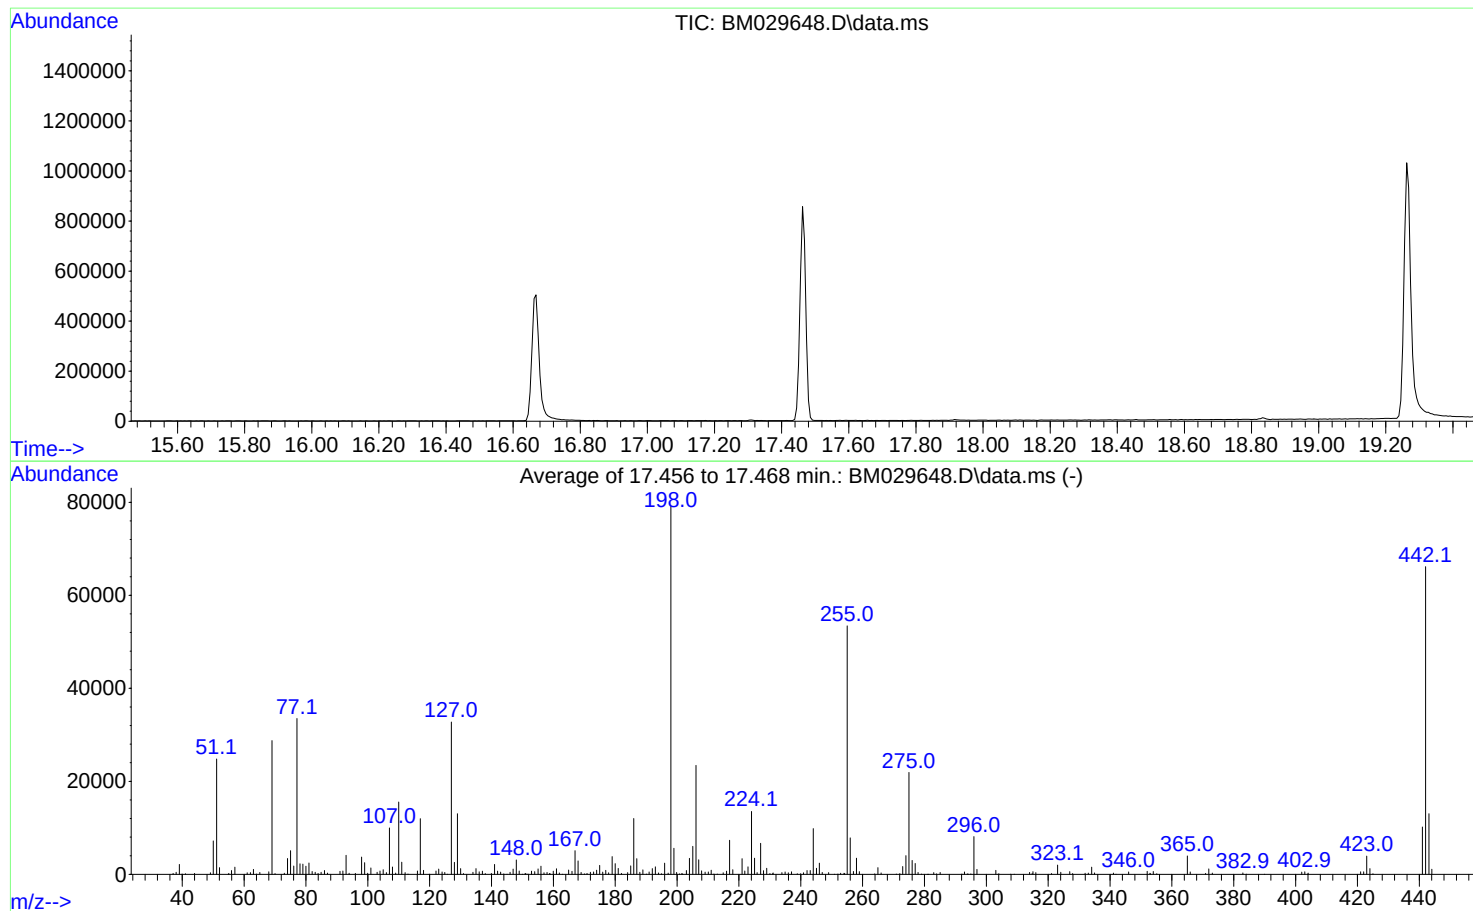




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	24819	PASS
68	69	0.00	2	1.9	540	PASS
69	198	0.00	100	36.4	28763	PASS
70	69	0.00	2	0.6	180	PASS
127	198	10	80	41.4	32768	PASS
197	198	0.00	2	0.4	295	PASS
198	198	100	100	100.0	79091	PASS
199	198	5	9	7.1	5616	PASS
275	198	10	60	27.7	21912	PASS
365	198	1	100	5.0	3963	PASS
441	198	0.01	100	12.9	10178	PASS
442	442	50	100	100.0	66152	PASS
443	442	15	24	19.7	13024	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042621\
 Data File : BM029648.D
 Acq On : 26 Apr 2021 13:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 26 14:29:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 22 15:55:11 2021
 Response via : Initial Calibration

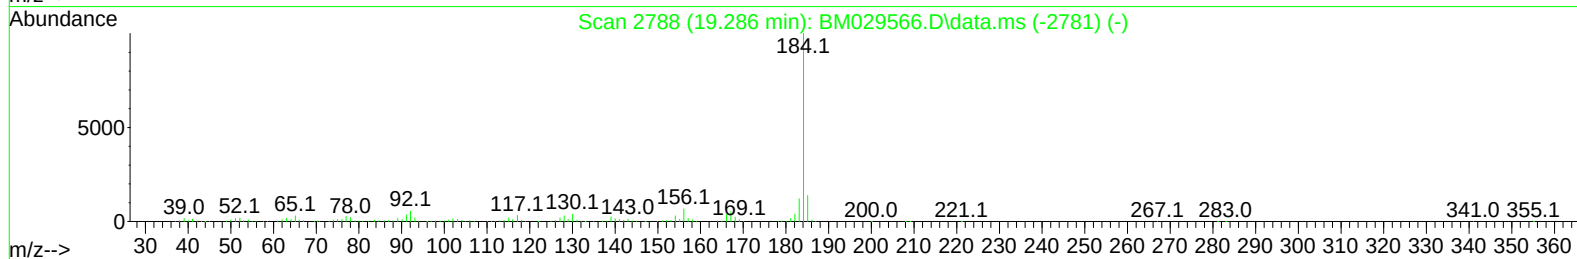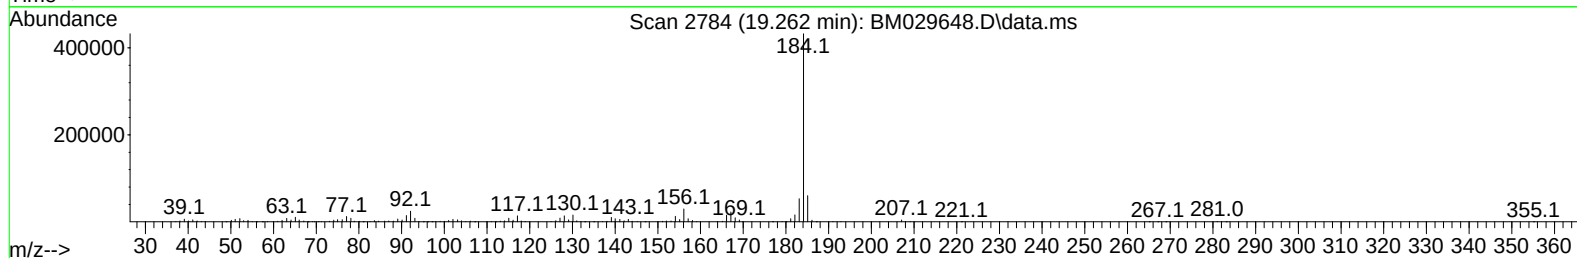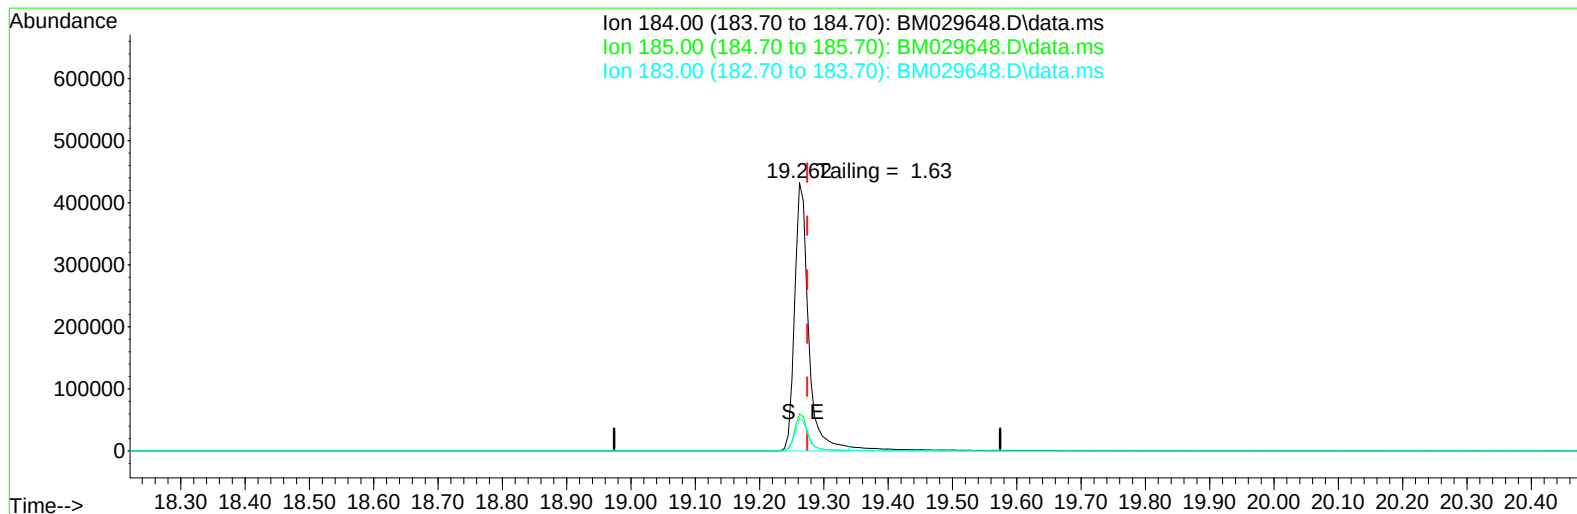

TIC: BM029648.D\data.ms

(77) Benzidine

19.262min (-0.012) 596763.26 ng




response 669648

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.92
183.00	12.30	12.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042621\
 Data File : BM029648.D
 Acq On : 26 Apr 2021 13:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Apr 26 14:29:24 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 22 15:55:11 2021
 Response via : Initial Calibration

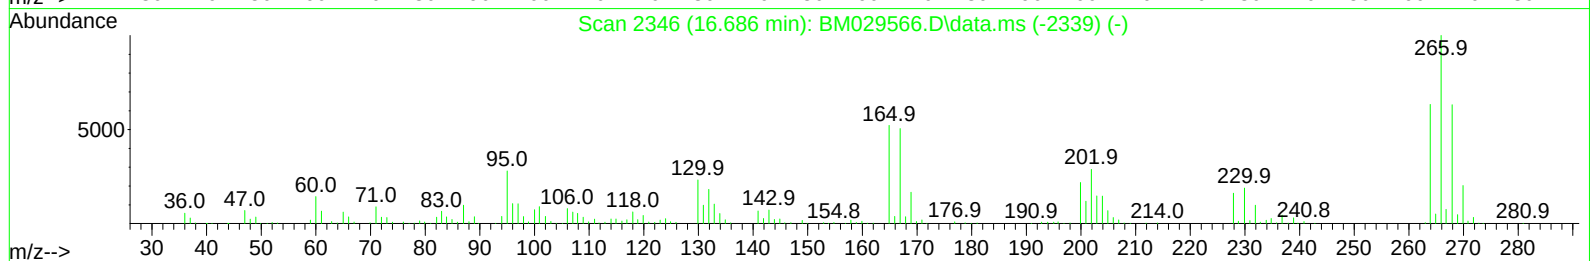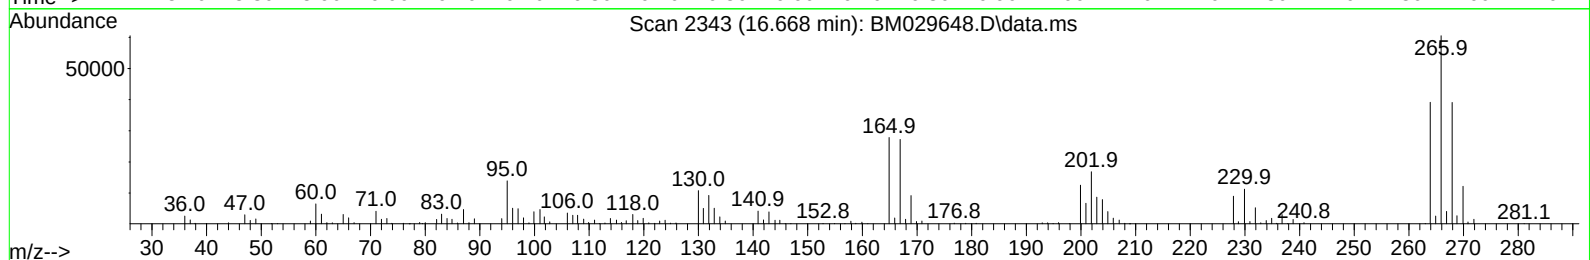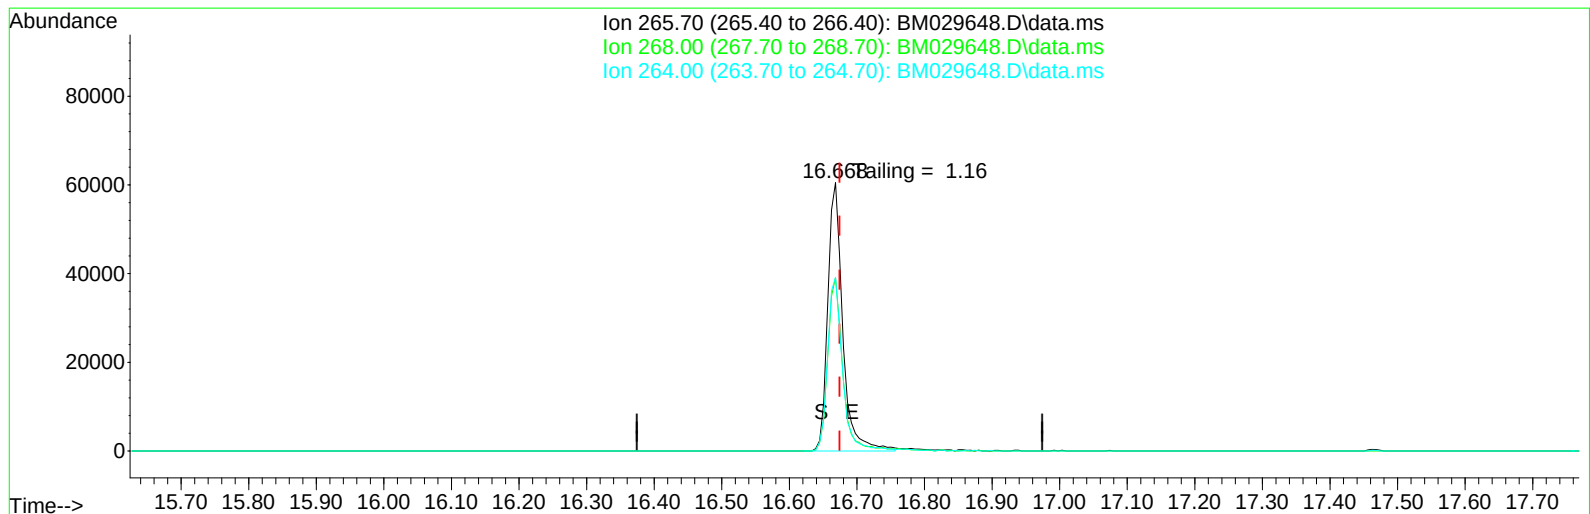

TIC: BM029648.D\data.ms

(70) Pentachlorophenol (C)

16.668min (-0.006) 0.00 ng

response 93548

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.00	64.64
264.00	64.90	64.69
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_M
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
4/26/2021	BNA_M	<u>BM029648.D</u>
Compound Name	Response	Retention Time
DDT	317233	20.49
DDD	1629	20.06
DDE	481	19.55
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2110	319343	0.66

Instrument :
BNA_M
ClientSampleId :
DFTPP