

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
 Data File : BM039672.D
 Acq On : 26 Apr 2023 11:15
 Operator : CG/JU
 Sample : PB152370BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK370

Quant Time: Apr 27 01:02:24 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Apr 26 19:06:24 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	4425	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.616	136	16563	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.468	164	9059	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.220	188	18951	0.400	ng/ul	-0.03
17) Chrysene-d12	21.440	240	11765	0.400	ng/ul	# 0.00
23) Perylene-d12	23.784	264	12725	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.209	96	34773	4.245	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.238	152	6561	0.343	ng/ul	0.00
18) Fluoranthene-d10	19.260	212	12566	0.343	ng/ul	-0.02
Target Compounds						
					Qvalue	
12) Fluorene	15.462	166	2372	0.086	ng/ul#	16
20) Pyrene	19.618	202	1936	0.035	ng/ul#	1
26) Benzo(a)pyrene	23.623	252	2907	0.071	ng/ul#	65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
Data File : BM039672.D
Acq On : 26 Apr 2023 11:15
Operator : CG/JU
Sample : PB152370BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK370

Quant Time: Apr 27 01:02:24 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 26 19:06:24 2023
Response via : Initial Calibration

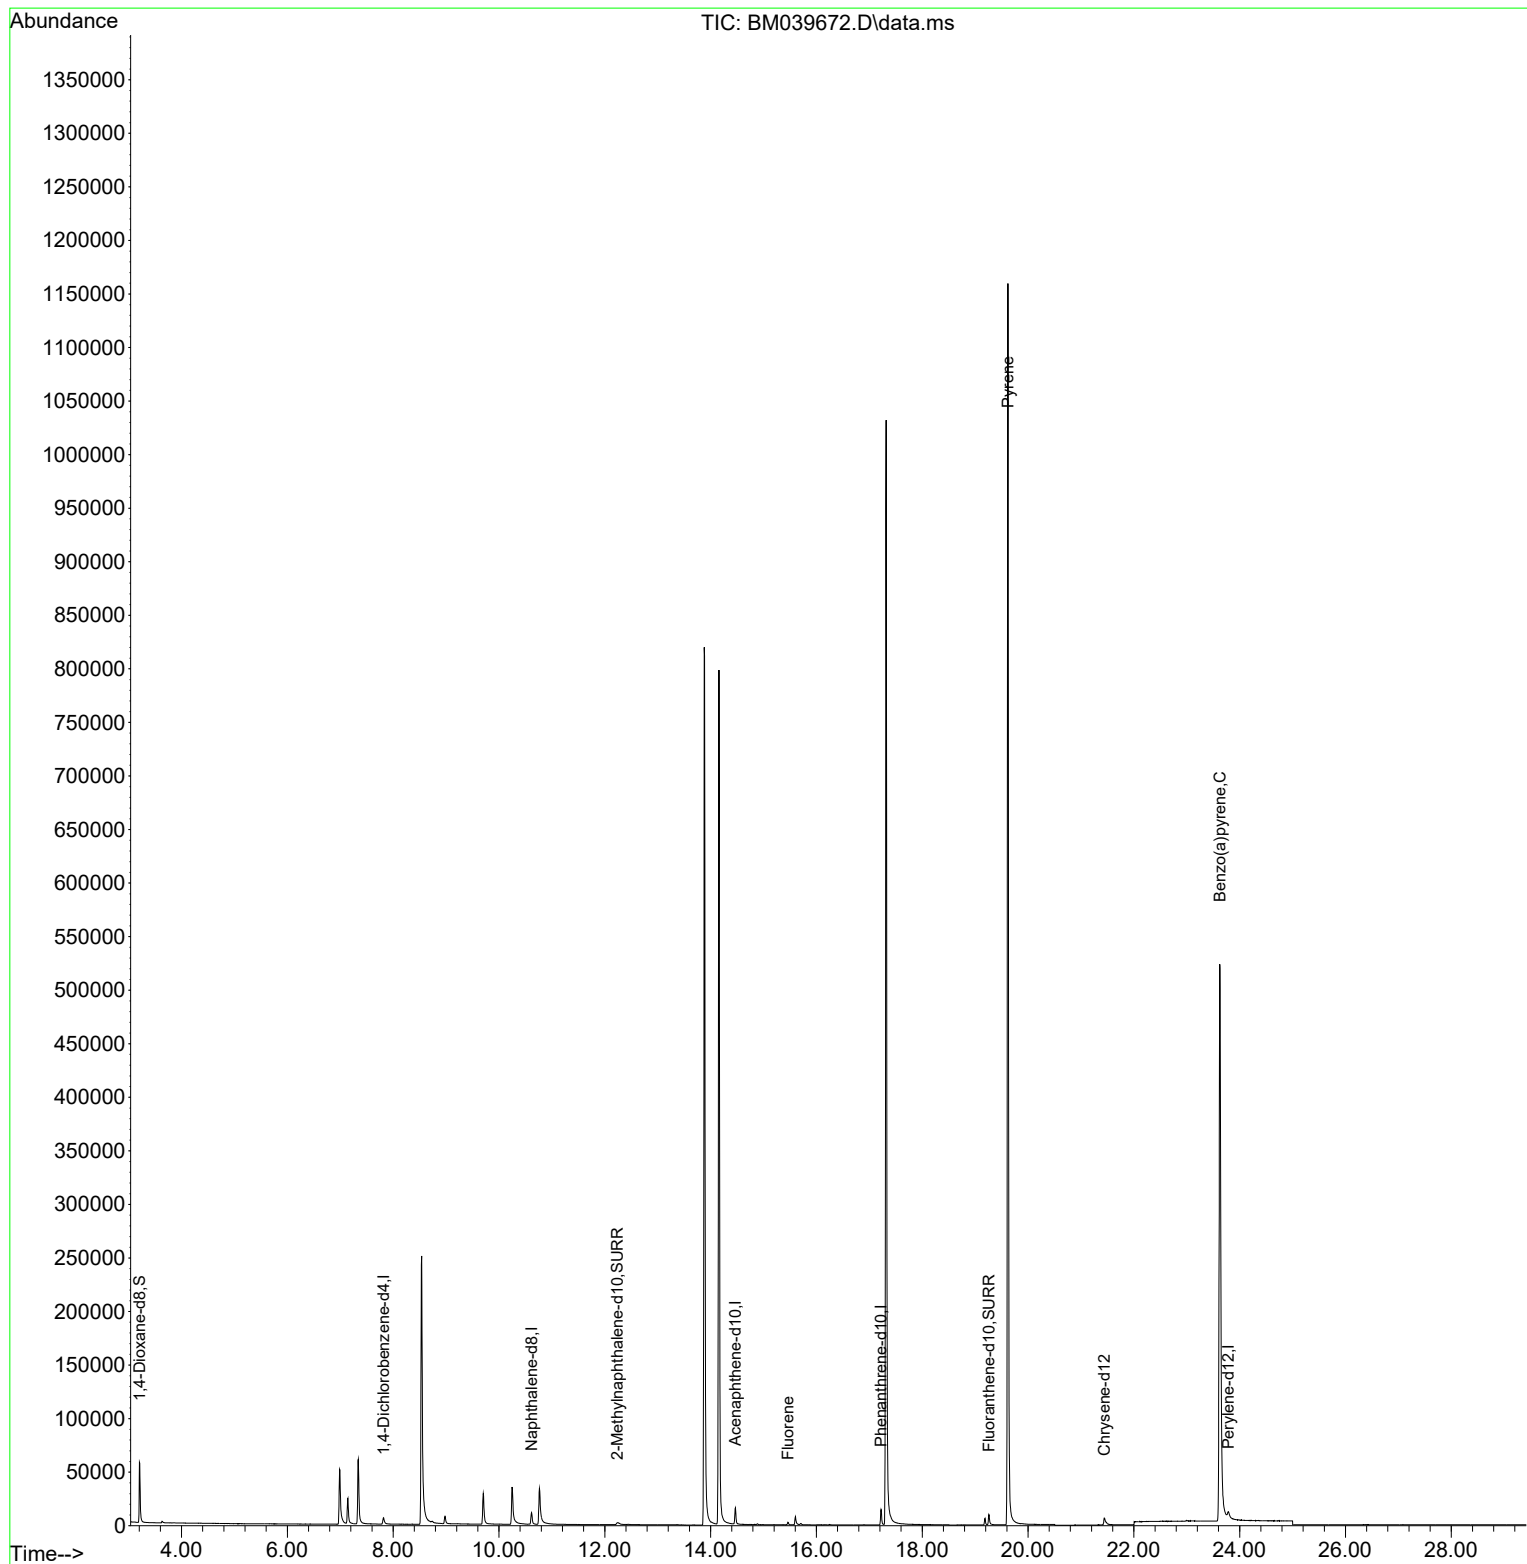

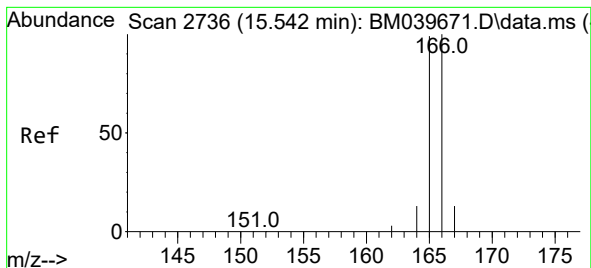

#12

Fluorene

Concen: 0.086 ng/ul

RT: 15.462 min Scan# 21

Delta R.T. -0.080 min

Lab File: BM039672.D

Acq: 26 Apr 2023 11:15

Instrument :

BNA_M

ClientSampleId :

SBLK370





Tgt Ion:166 Resp: 2372

Ion Ratio Lower Upper

166 100

165 9.1 77.8 116.8#

167 33.8 11.8 17.6#

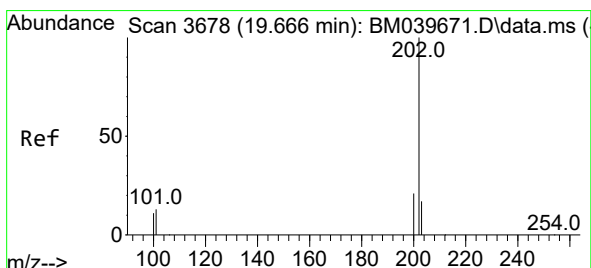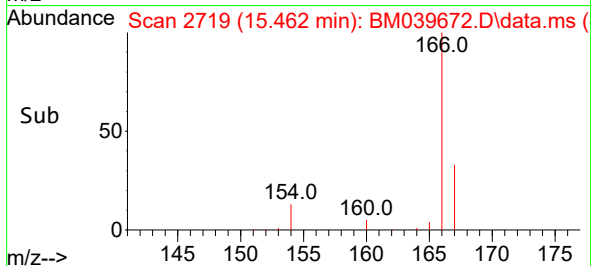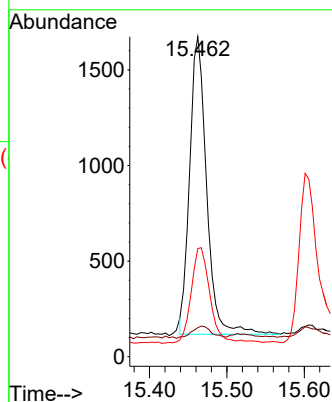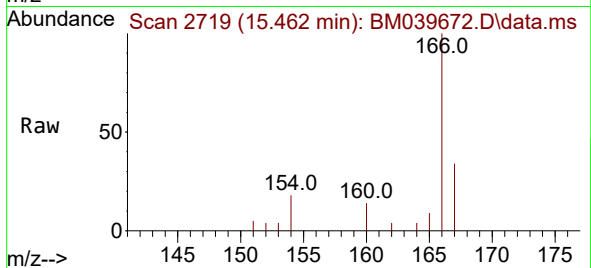

#20

Pyrene

Concen: 0.035 ng/ul

RT: 19.618 min Scan# 3668

Delta R.T. -0.048 min

Lab File: BM039672.D

Acq: 26 Apr 2023 11:15




Tgt Ion:202 Resp: 1936


Ion Ratio Lower Upper

202 100

101 174.6 11.1 16.7#


100 1327.4 8.8 13.2#

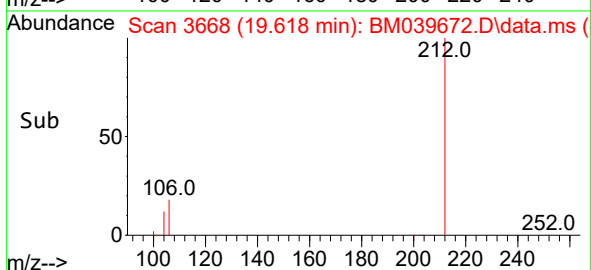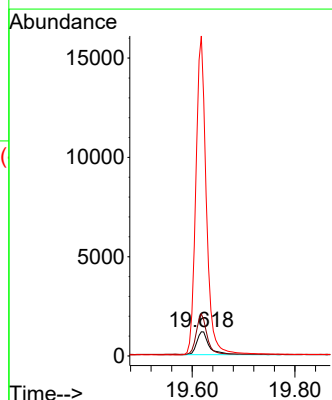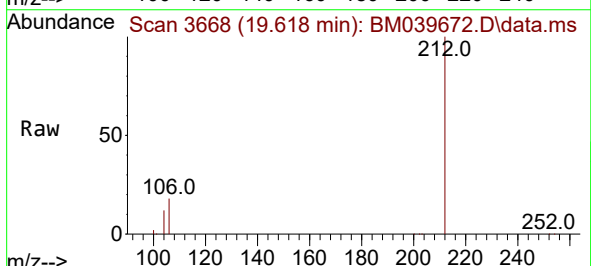

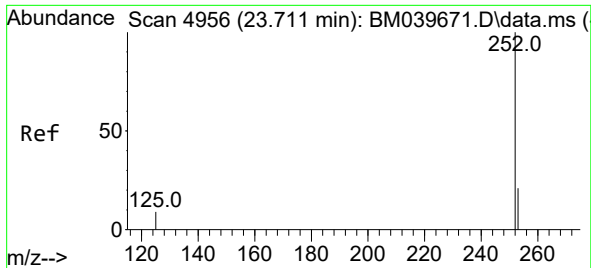

#26
Benzo(a)pyrene
Concen: 0.071 ng/ul
RT: 23.623 min Scan# 4956
Delta R.T. -0.088 min
Lab File: BM039672.D
Acq: 26 Apr 2023 11:15

Instrument :
BNA_M
ClientSampleId :
SBLK370

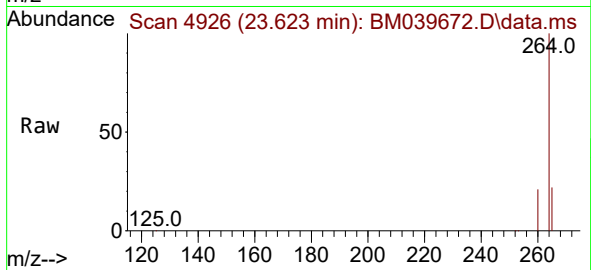

Tgt Ion:252 Resp: 2907
Ion Ratio Lower Upper
252 100
253 57.5 31.0 46.4#
125 58.2 28.2 42.4#

